

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010819\
 Data File : BF111926.D
 Acq On : 8 Jan 2019 23:55
 Operator : JU/SJ
 Sample : K1075-13 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jan 09 01:00:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 07 14:33:51 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	127676	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	444857	20.00	ng	0.00
39) Acenaphthene-d10	9.93	164	162433	20.00	ng	0.00
64) Phenanthrene-d10	11.41	188	321078	20.00	ng	0.00
76) Chrysene-d12	14.06	240	204404	20.00	ng	0.00
87) Perylene-d12	15.54	264	206375	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	457776	61.34	ng	0.00
7) Phenol-d6	6.53	99	539255	56.06	ng	0.00
23) Nitrobenzene-d5	7.45	82	322484	38.74	ng	-0.01
42) 2,4,6-Tribromophenol	10.72	330	108605	51.40	ng	0.00
45) 2-Fluorobiphenyl	9.24	172	458763	41.18	ng	-0.01
79) Terphenyl-d14	12.99	244	408370	37.92	ng	0.00
Target Compounds						
9) Benzaldehyde	6.53	77	1354	Below Cal	Qvalue	# 1
10) Phenol	6.54	94	26514	2.536 ng		80
19) n-Nitroso-di-n-propylamine	7.44	70	41838	6.694 ng	#	81
25) Isophorone	7.45	82	322478	23.925 ng	#	65
50) Dimethylphthalate	9.63	163	62938	5.158 ng		97
57) 2,4-Dinitrotoluene	9.93	165	20119	5.706 ng	#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010819\
Data File : BF111926.D
Acq On : 8 Jan 2019 23:55
Operator : JU/SJ
Sample : K1075-13 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jan 09 01:00:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 07 14:33:51 2019
Response via : Initial Calibration

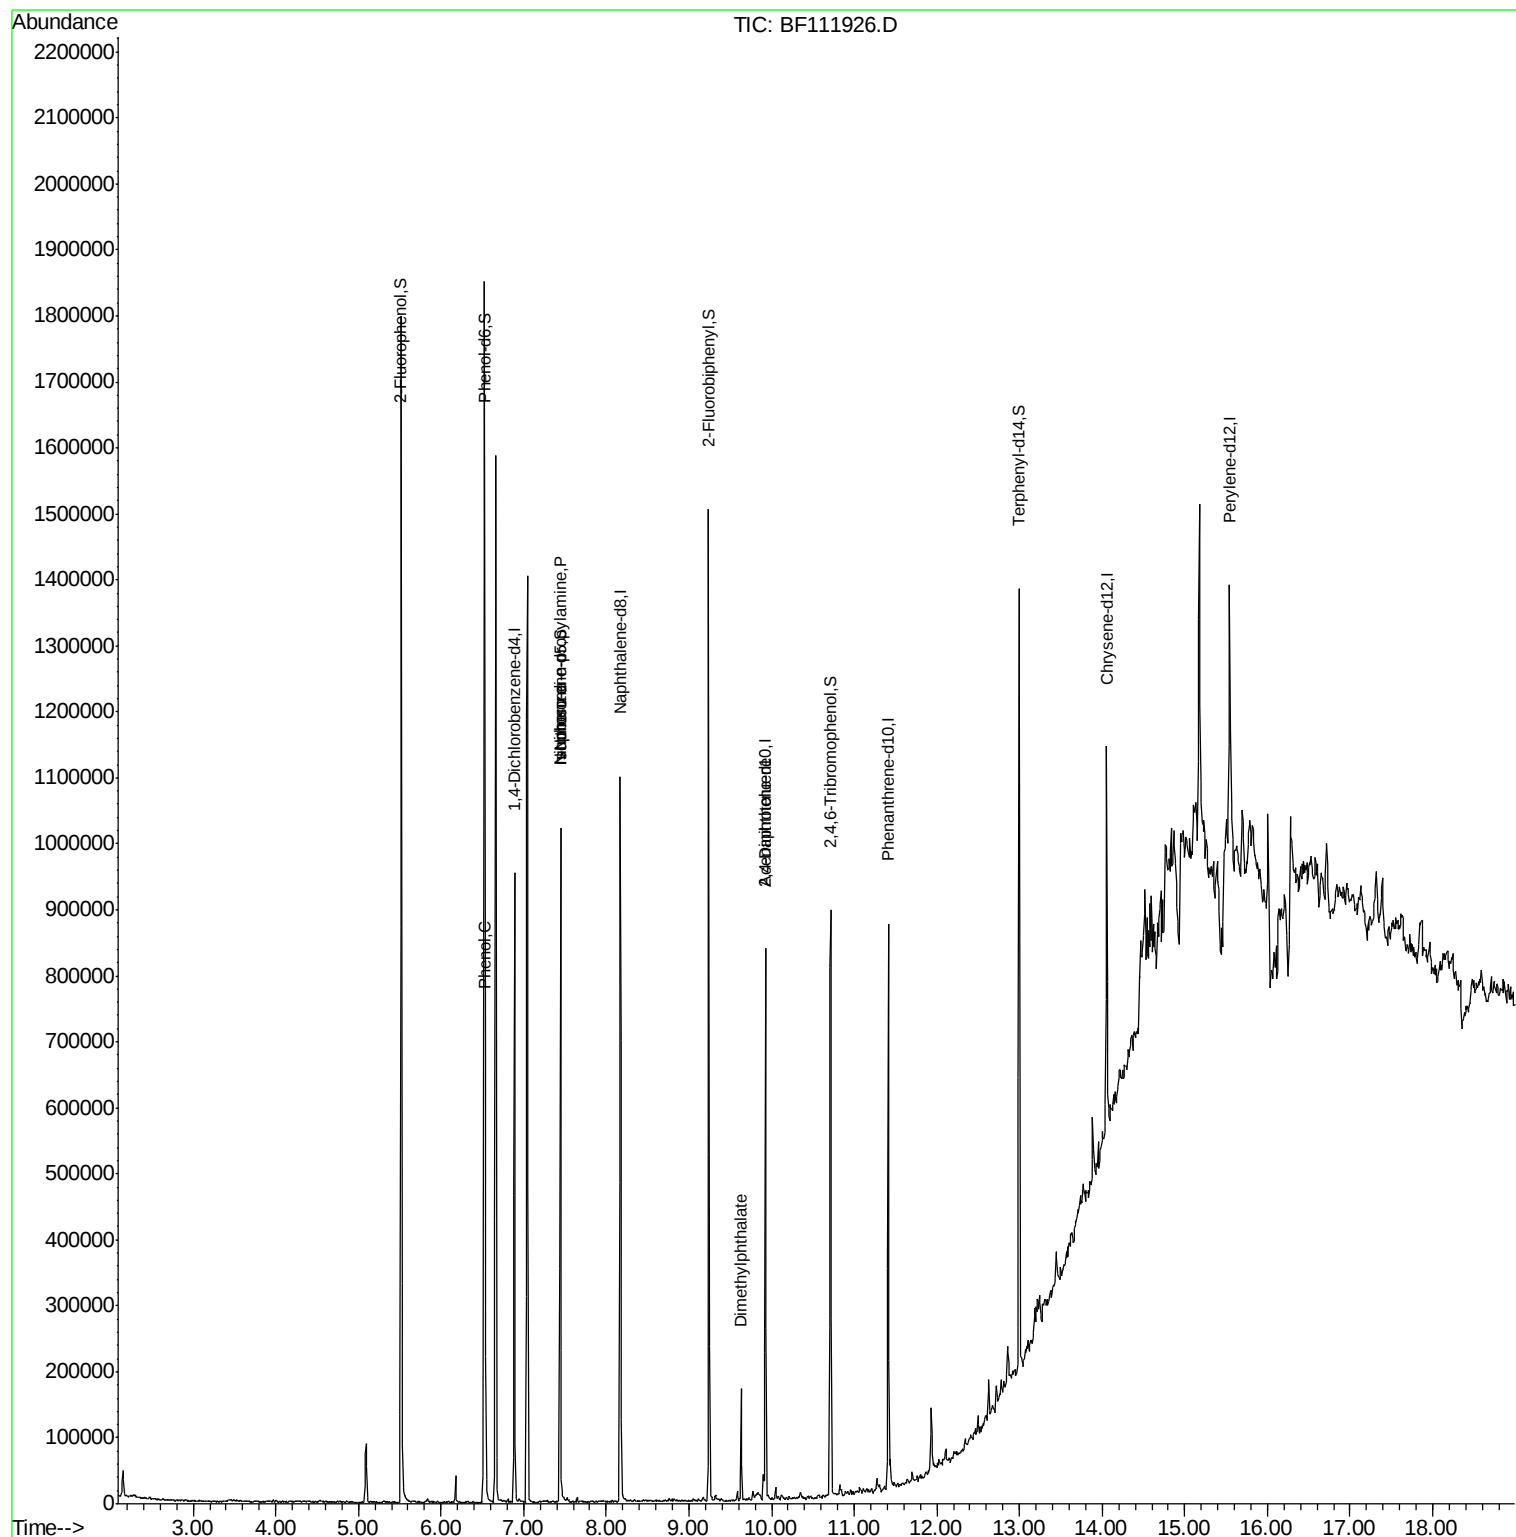

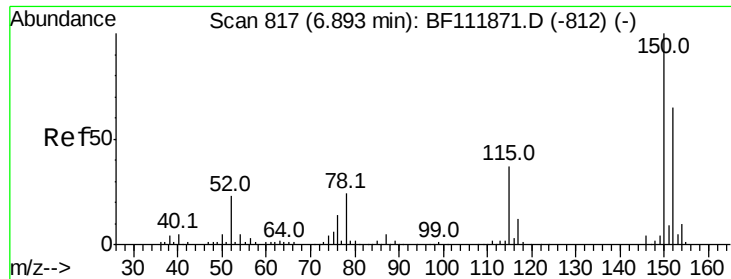


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.89 min Scan# 816
Delta R.T. -0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 127676
Ion Ratio Lower Upper
152 100
150 156.8 122.7 184.1
115 59.1 45.2 67.8

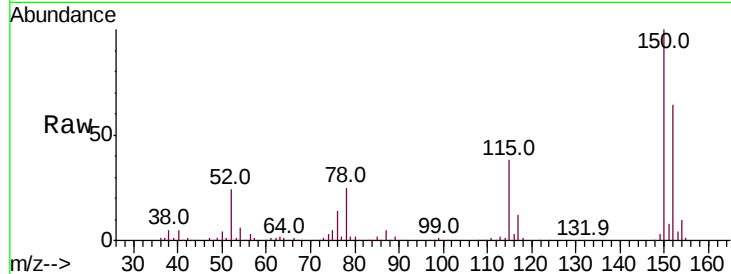


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

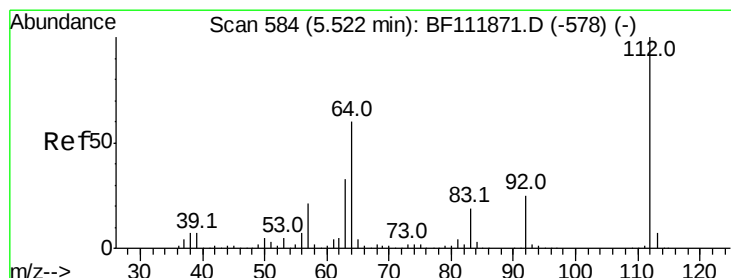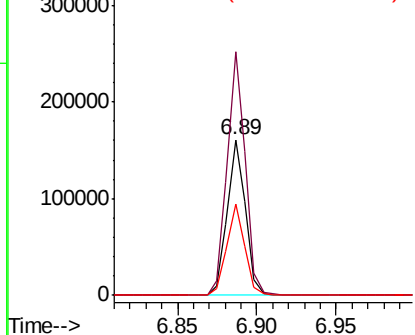



#5


2-Fluorophenol
Concen: 61.340 ng
RT: 5.52 min Scan# 583
Delta R.T. -0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Tgt Ion:112 Resp: 457776
Ion Ratio Lower Upper
112 100
64 63.0 48.3 72.5
63 33.7 26.1 39.1

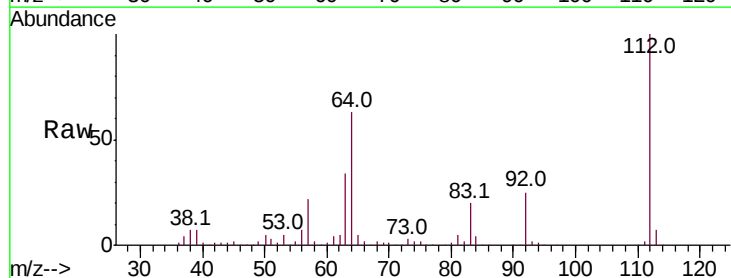

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

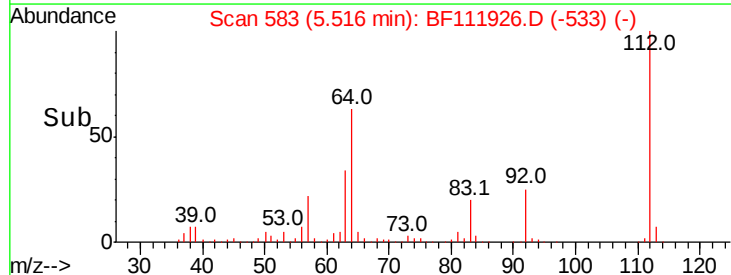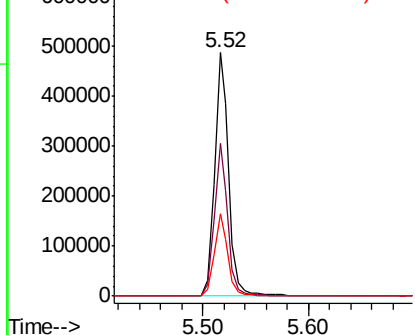

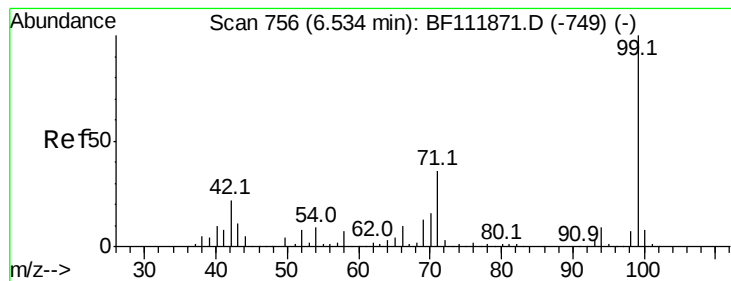

#7

Phenol-d6

Concen: 56.063 ng

RT: 6.53 min Scan# 755

Delta R.T. -0.01 min

Lab File: BF111926.D

Acq: 8 Jan 2019 23:55

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 539255

Ion Ratio Lower Upper




99 100

42 21.0 17.9 26.9

71 35.5 28.7 43.1

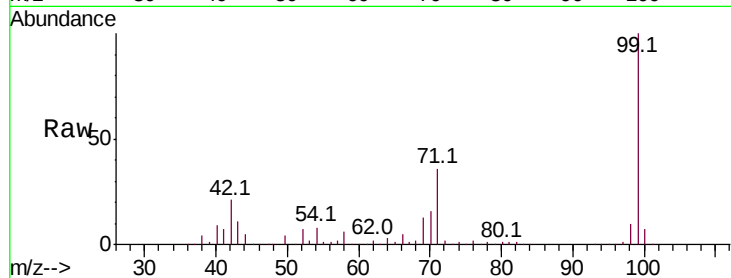

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

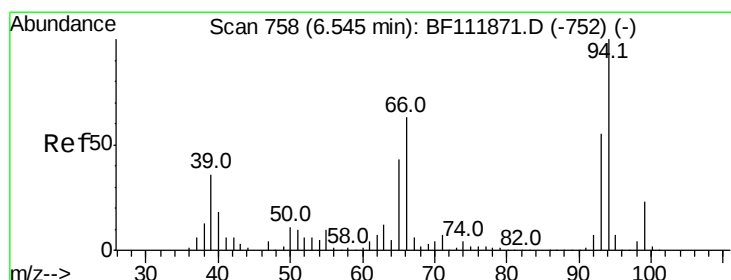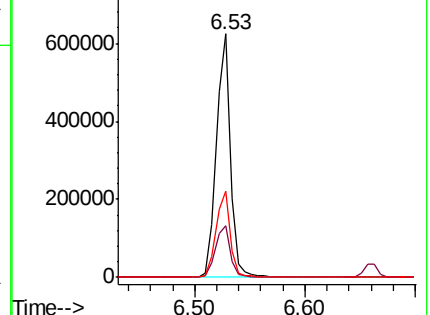

#10

Phenol

Concen: 2.536 ng

RT: 6.54 min Scan# 757

Delta R.T. -0.01 min

Lab File: BF111926.D

Acq: 8 Jan 2019 23:55


Tgt Ion: 94 Resp: 26514

Ion Ratio Lower Upper



94 100


65 30.0 22.8 62.8

66 48.3 43.3 83.3

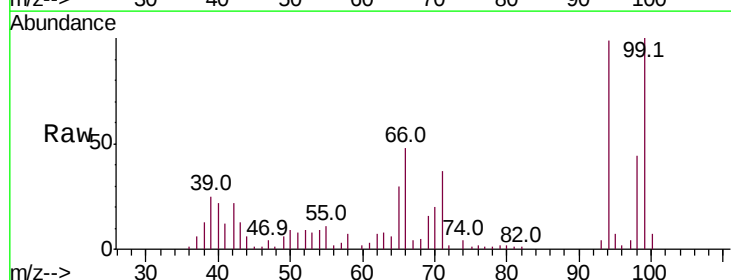

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



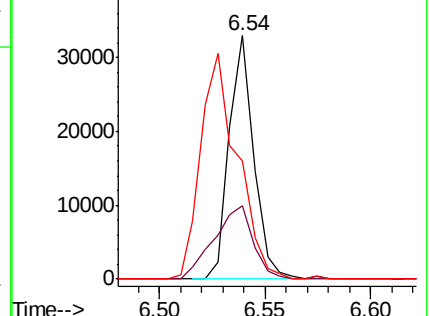
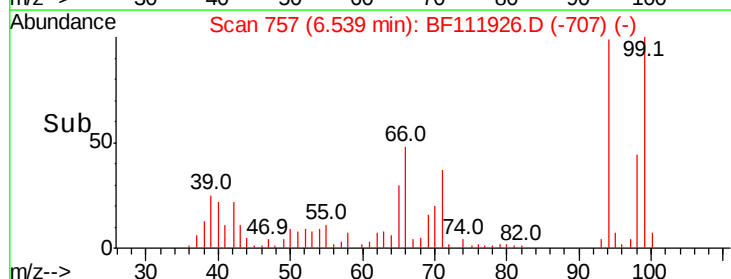


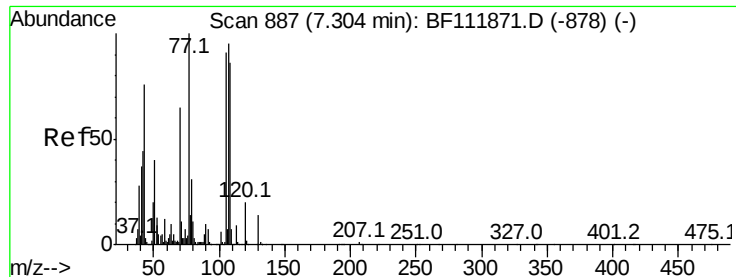

#19
n-Nitroso-di-n-propylamine
Concen: 6.694 ng
RT: 7.44 min Scan# 910
Delta R.T. 0.14 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
70	100		
42	57.7	53.6	80.4
101	0.0	7.3	10.9#
130	2.5	16.8	25.2#

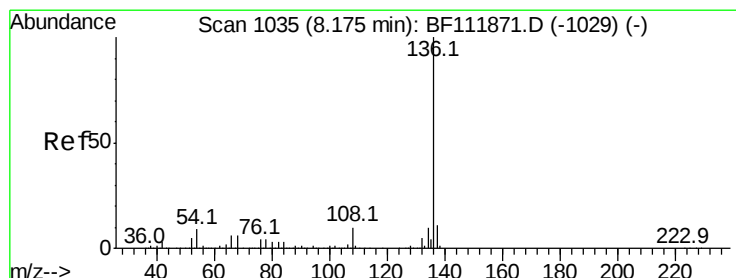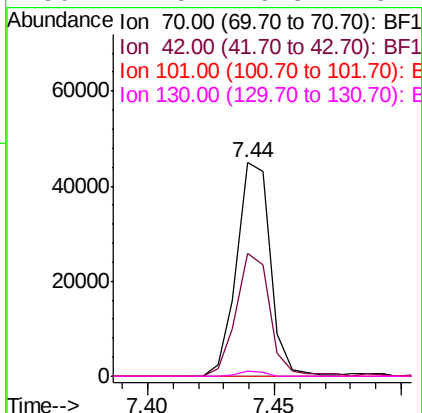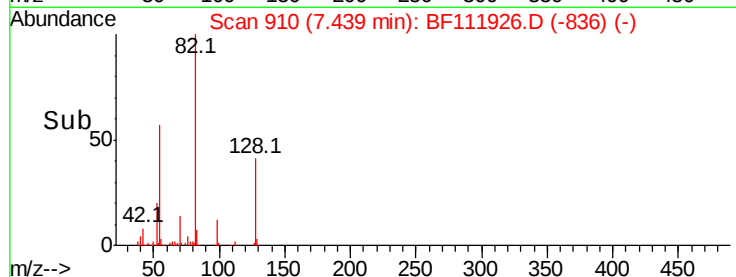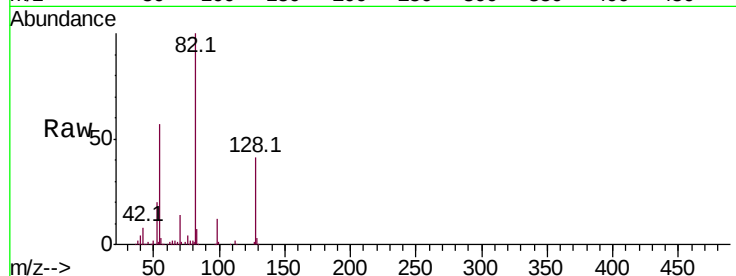

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.17 min Scan# 1034
Delta R.T. -0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.1	13.7
54	8.6	7.2	10.8
68	5.6	4.4	6.6

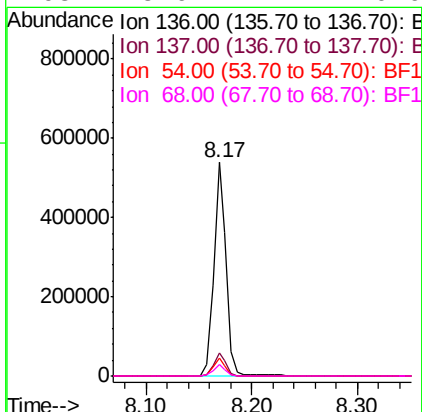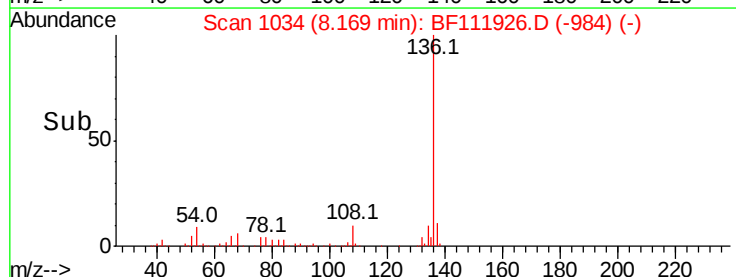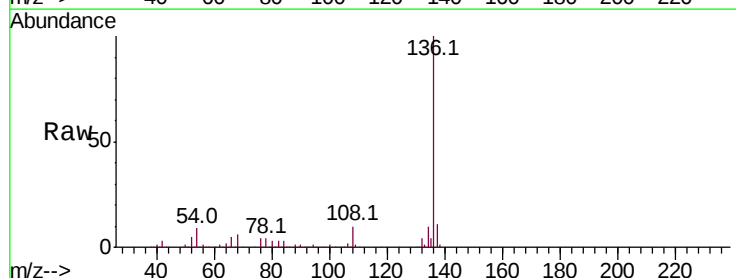







#23
 Nitrobenzene-d5
 Concen: 38.743 ng
 RT: 7.45 min Scan# 911
 Delta R.T. -0.01 min
 Lab File: BF111926.D
 Acq: 8 Jan 2019 23:55

Instrument :
 BNA_F
 ClientSampleID :

Tot Ion: 82 Resp: 322484
 Ion Ratio Lower Upper
 82 100
 128 46.8 35.7 53.5
 54 52.8 45.8 68.8

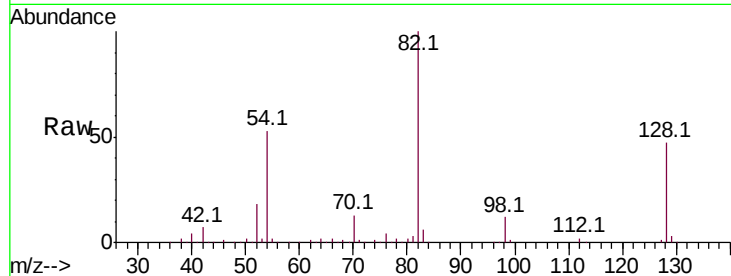


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

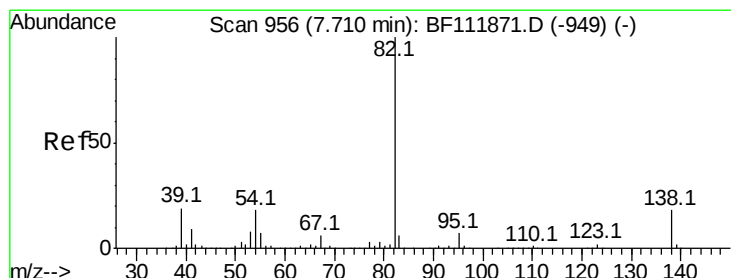
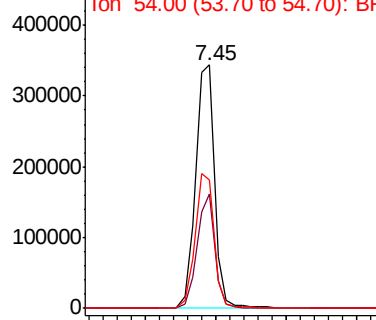



#25
 Isophorone
 Concen: 23.925 ng
 RT: 7.45 min Scan# 911
 Delta R.T. -0.26 min
 Lab File: BF111926.D
 Acq: 8 Jan 2019 23:55

Tgt Ion: 82 Resp: 322478
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.8 8.6#
 138 0.0 14.4 21.6#

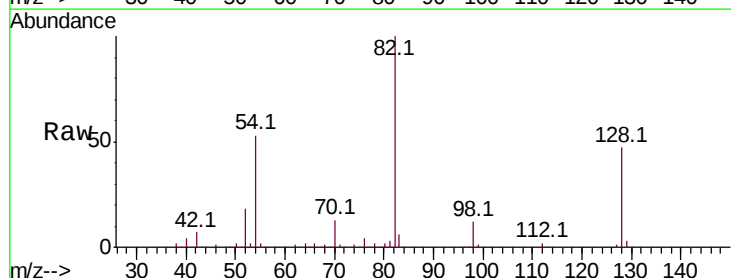

Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 95.00 (94.70 to 95.70): BF1
 Ion 138.00 (137.70 to 138.70): BF1

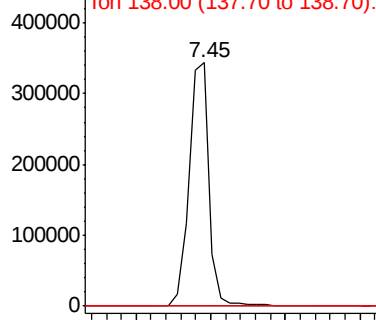


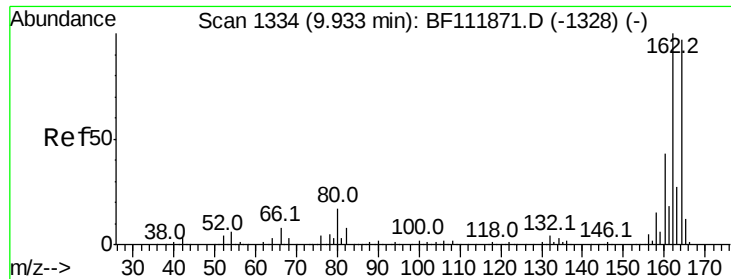




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.93 min Scan# 1333
Delta R.T. -0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion:164 Resp: 162433
Ion Ratio Lower Upper
164 100
162 103.4 82.2 123.2
160 45.0 35.5 53.3

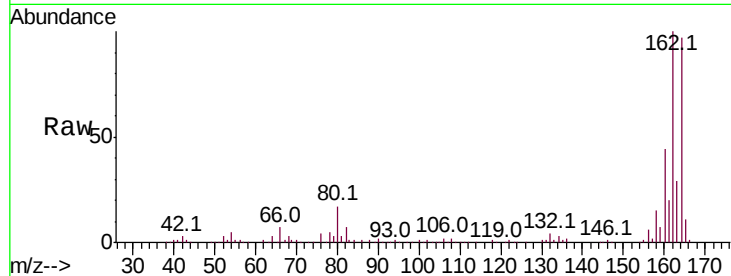


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

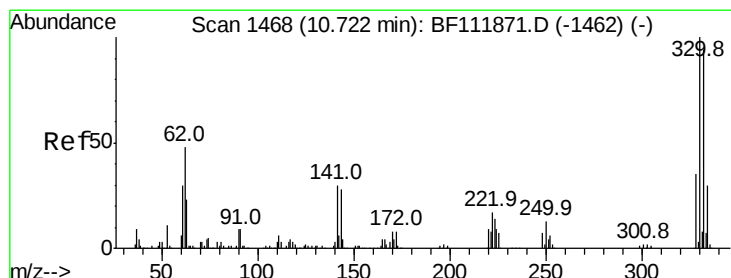
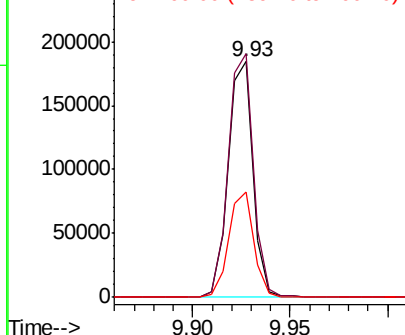



#42
2,4,6-Tribromophenol
Concen: 51.404 ng
RT: 10.72 min Scan# 1467
Delta R.T. -0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Tgt Ion:330 Resp: 108605
Ion Ratio Lower Upper
330 100
332 96.0 76.9 115.3
141 30.7 23.7 35.5

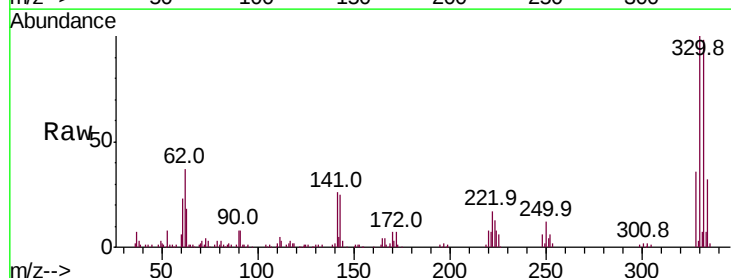

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

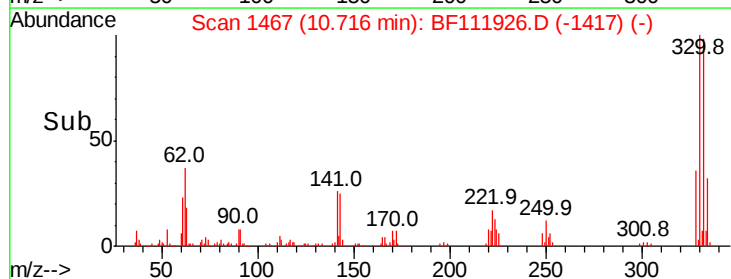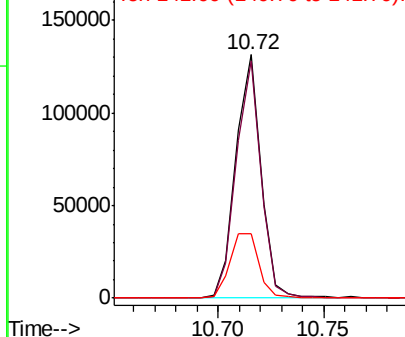


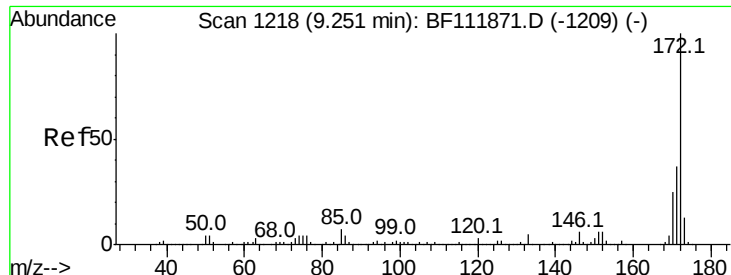




#45
2-Fluorobiphenyl
Concen: 41.184 ng
RT: 9.24 min Scan# 1216
Delta R.T. -0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 458763
Ion Ratio Lower Upper
172 100
171 34.6 29.6 44.4
170 22.8 19.8 29.8

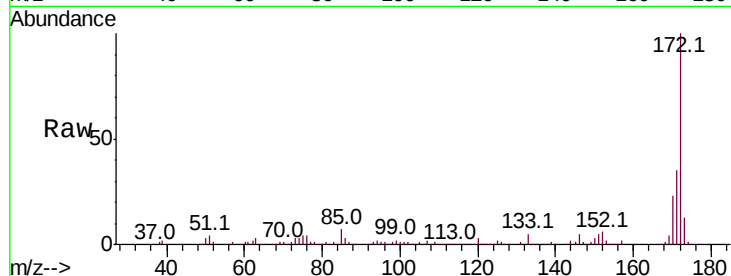


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

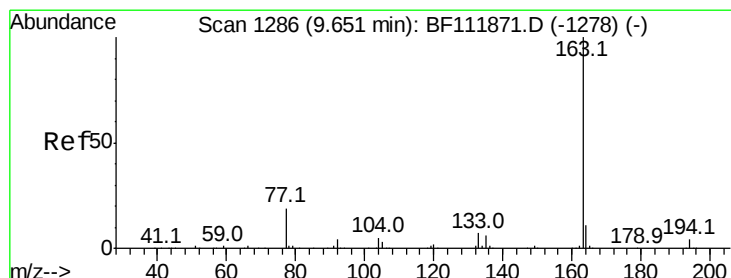
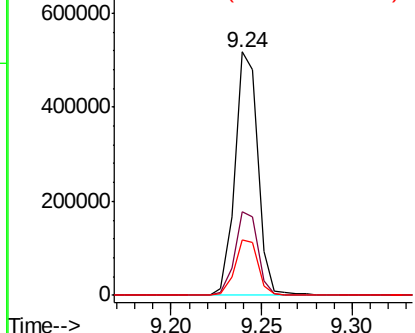



#50
Dimethylphthalate
Concen: 5.158 ng
RT: 9.63 min Scan# 1283
Delta R.T. -0.02 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Tgt Ion:163 Resp: 62938
Ion Ratio Lower Upper
163 100
194 4.6 3.4 5.2
164 9.0 8.5 12.7

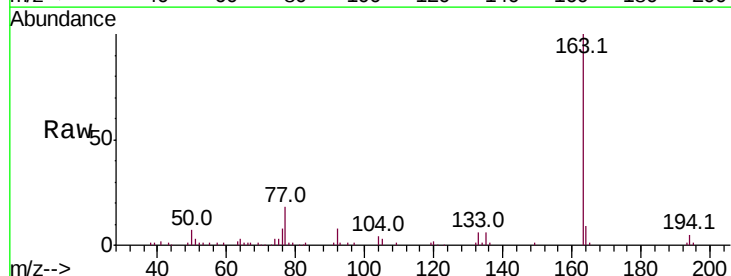

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

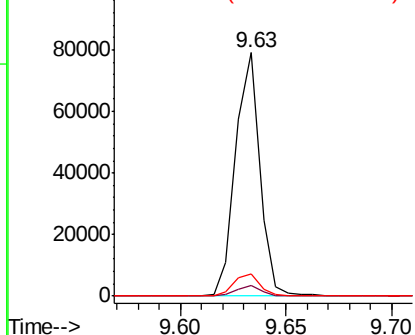


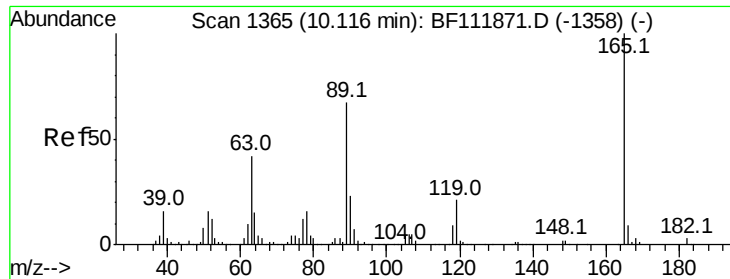

#57
 2,4-Dinitrotoluene
 Concen: 5.706 ng
 RT: 9.93 min Scan# 1333
 Delta R.T. -0.19 min
 Lab File: BF111926.D
 Acq: 8 Jan 2019 23:55

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.6	34.1	51.1#
89	1.5	53.5	80.3#
182	0.0	2.0	3.0#



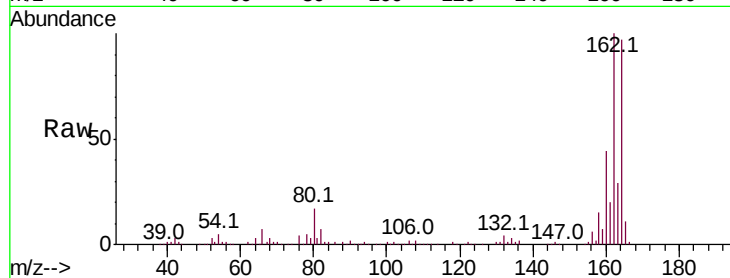


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

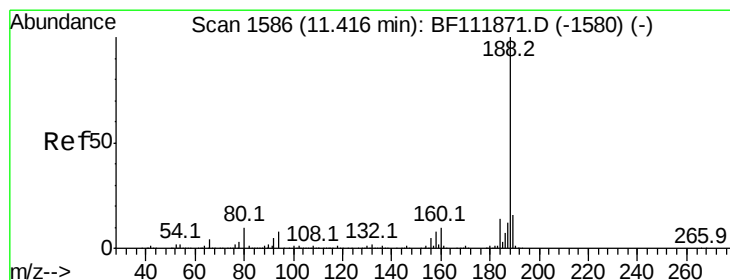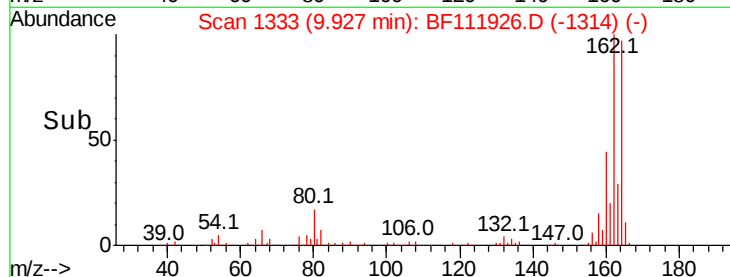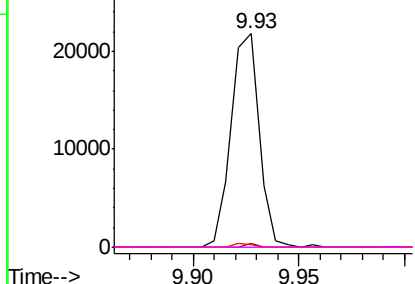

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.41 min Scan# 1585
 Delta R.T. -0.01 min
 Lab File: BF111926.D
 Acq: 8 Jan 2019 23:55



Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.9	6.6	10.0
80	9.9	7.7	11.5

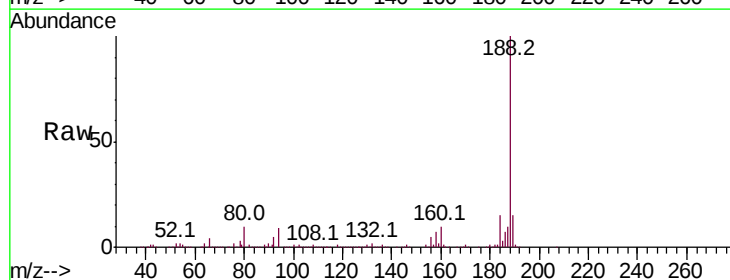


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1



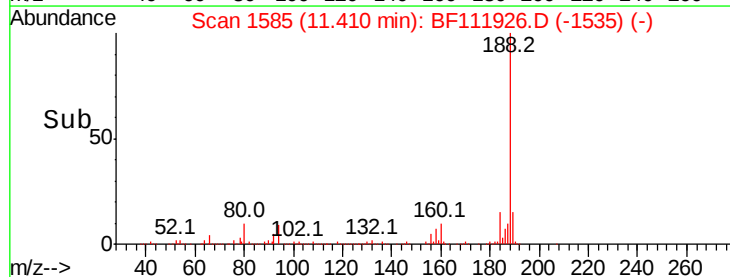
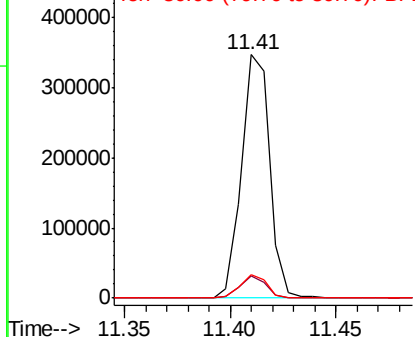


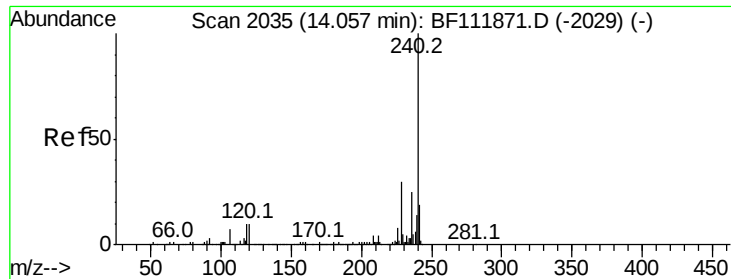

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.06 min Scan# 2035
Delta R.T. -0.00 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
240	100		
120	9.7	8.2	12.2
236	24.7	20.2	30.4

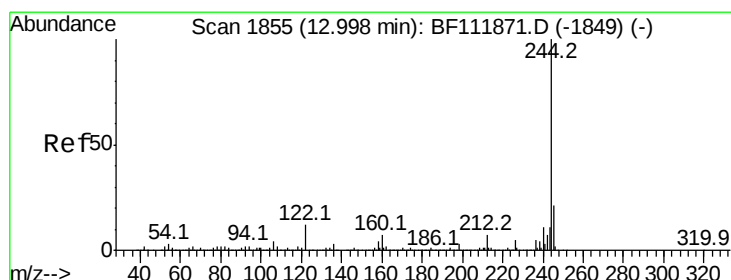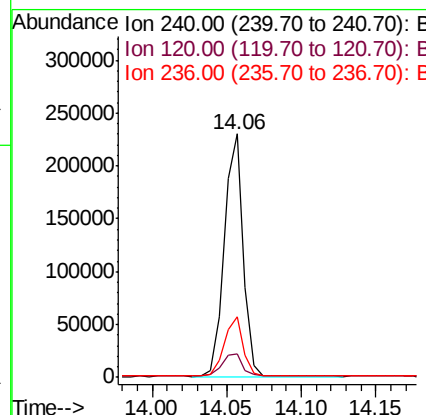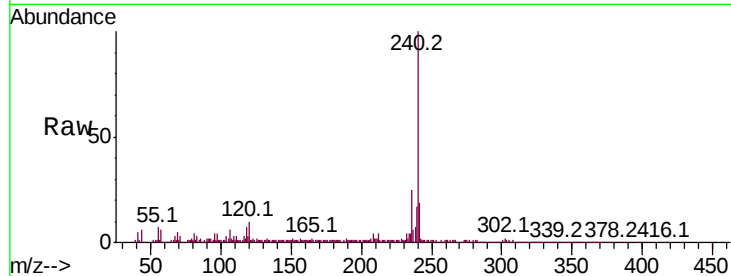

#79
Terphenyl-d14
Concen: 37.924 ng
RT: 12.99 min Scan# 1854
Delta R.T. -0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.7	5.8	8.8
122	10.9	9.5	14.3

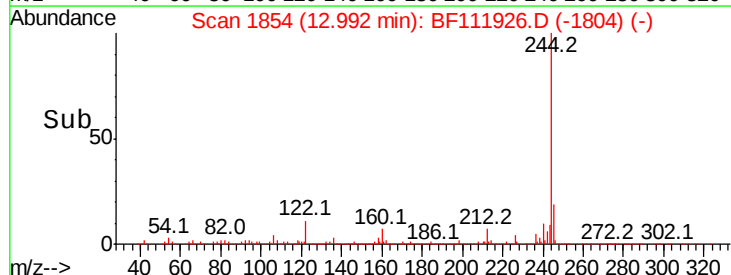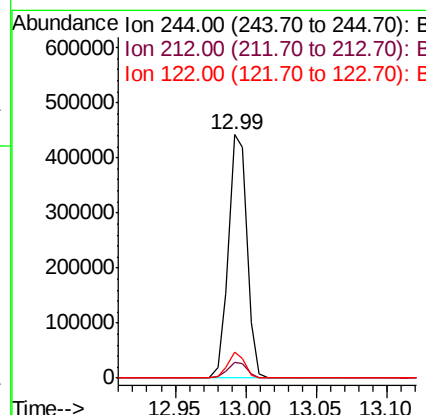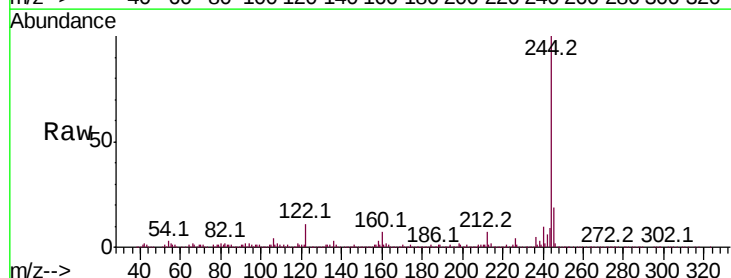



#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.54 min Scan# 2288
Delta R.T. 0.01 min
Lab File: BF111926.D
Acq: 8 Jan 2019 23:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.2	28.8
265	22.5	17.1	25.7

