

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010819\
 Data File : BF111908.D
 Acq On : 8 Jan 2019 15:47
 Operator : JU/SJ
 Sample : K1012-05RE 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EO-02-010419-CRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	10	14	18	rBV	74226	86674	2.21%	0.275%
2	5.093	507	511	520	rVB	79847	87238	2.23%	0.276%
3	5.516	579	583	597	rVB	1654400	1496872	38.18%	4.742%
4	6.522	750	754	765	rBV	1736584	1480538	37.76%	4.690%
5	6.657	773	777	780	rBV	1984392	1635098	41.71%	5.180%
6	6.881	812	815	819	rBV	1084392	964500	24.60%	3.056%
7	7.040	838	842	846	rBV	1487623	1209172	30.84%	3.831%
8	7.440	905	910	913	rBV	1140393	967264	24.67%	3.064%
9	8.163	1028	1033	1037	rBV	1095693	1036219	26.43%	3.283%
10	8.757	1131	1134	1137	rBV	75260	59476	1.52%	0.188%
11	9.239	1212	1216	1219	rBV	1385652	1243037	31.71%	3.938%
12	9.322	1226	1230	1235	rBV2	90438	83526	2.13%	0.265%
13	9.628	1279	1282	1287	rBV2	94078	94545	2.41%	0.300%
14	9.781	1305	1308	1312	rBV	53902	59863	1.53%	0.190%
15	9.851	1317	1320	1323	rVB	98151	79488	2.03%	0.252%
16	9.922	1328	1332	1335	rVB	1013356	874778	22.31%	2.771%
17	10.122	1362	1366	1371	rVB2	36804	45919	1.17%	0.145%
18	10.351	1398	1405	1407	rBV	103821	97950	2.50%	0.310%
19	10.463	1421	1424	1430	rBV	57535	63242	1.61%	0.200%
20	10.569	1437	1442	1448	rBV	36173	59832	1.53%	0.190%
21	10.704	1460	1465	1469	rBV	869570	766166	19.54%	2.427%
22	10.822	1479	1485	1491	rBV2	113169	149008	3.80%	0.472%
23	11.269	1555	1561	1564	rBV	86255	90637	2.31%	0.287%
24	11.298	1564	1566	1572	rVB	59729	69651	1.78%	0.221%
25	11.404	1580	1584	1586	rBV	930371	797864	20.35%	2.528%
26	11.427	1586	1588	1591	rVV	345360	274249	7.00%	0.869%
27	11.480	1594	1597	1600	rVB	93960	79961	2.04%	0.253%
28	11.698	1631	1634	1636	rBV2	73356	61883	1.58%	0.196%
29	11.798	1647	1651	1654	rBV	1381925	1219437	31.10%	3.863%
30	11.904	1667	1669	1671	rBV	52040	53826	1.37%	0.171%
31	11.927	1671	1673	1680	rVB2	213906	212445	5.42%	0.673%
32	12.022	1685	1689	1691	rBV	96111	106765	2.72%	0.338%
33	12.104	1700	1703	1706	rVB	64775	60923	1.55%	0.193%
34	12.198	1717	1719	1721	rBV2	54593	46232	1.18%	0.146%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010819\
Data File : BF111908.D
Acq On : 8 Jan 2019 15:47
Operator : JU/SJ
Sample : K1012-05RE 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-02-010419-CRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.457	1760	1763	1764	rBV	59110	54452	1.39%	0.173%
36	12.486	1764	1768	1769	rVV	3811869	3704298	94.48%	11.735%
37	12.504	1769	1771	1778	rVV	3924090	3920602	100.00%	12.421%
38	12.586	1782	1785	1788	rBV	661573	518289	13.22%	1.642%
39	12.616	1788	1790	1796	rVV	518673	516177	13.17%	1.635%
40	12.663	1796	1798	1804	rVV7	38337	68963	1.76%	0.218%
41	12.716	1804	1807	1810	rVV2	96338	98582	2.51%	0.312%
42	12.822	1822	1825	1827	rBV2	131101	143569	3.66%	0.455%
43	12.845	1827	1829	1836	rVB	460979	476379	12.15%	1.509%
44	12.986	1850	1853	1856	rVB	1365984	1106123	28.21%	3.504%
45	13.145	1877	1880	1882	rBV4	108445	107540	2.74%	0.341%
46	13.174	1882	1885	1890	rVV	152343	181434	4.63%	0.575%
47	13.239	1890	1896	1899	rVB3	136731	223485	5.70%	0.708%
48	13.310	1906	1908	1910	rBV	75881	62572	1.60%	0.198%
49	13.369	1916	1918	1921	rBV	75417	72173	1.84%	0.229%
50	13.886	2003	2006	2010	rVB3	100883	122648	3.13%	0.389%
51	13.980	2020	2022	2025	rVB3	71845	52473	1.34%	0.166%
52	14.045	2028	2033	2036	rVV2	1220511	1392482	35.52%	4.411%
53	14.069	2036	2037	2043	rVB	264724	199834	5.10%	0.633%
54	14.204	2058	2060	2063	rBV2	66824	46461	1.19%	0.147%
55	14.821	2163	2165	2168	rBV2	112321	100354	2.56%	0.318%
56	15.098	2208	2212	2220	rVB	296892	591481	15.09%	1.874%
57	15.163	2221	2223	2227	rVB2	107592	107499	2.74%	0.341%
58	15.398	2261	2263	2269	rVB	157453	210620	5.37%	0.667%
59	15.468	2271	2275	2277	rVV	206640	257176	6.56%	0.815%
60	15.533	2281	2286	2297	rVB	764452	1360235	34.69%	4.309%
61	15.927	2351	2353	2354	rBV2	77025	47234	1.20%	0.150%
62	16.657	2474	2477	2479	rBV3	78294	107618	2.74%	0.341%


Sum of corrected areas: 31565031

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010819\
Data File : BF111908.D
Acq On : 8 Jan 2019 15:47
Operator : JU/SJ
Sample : K1012-05RE 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-02-010419-CRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

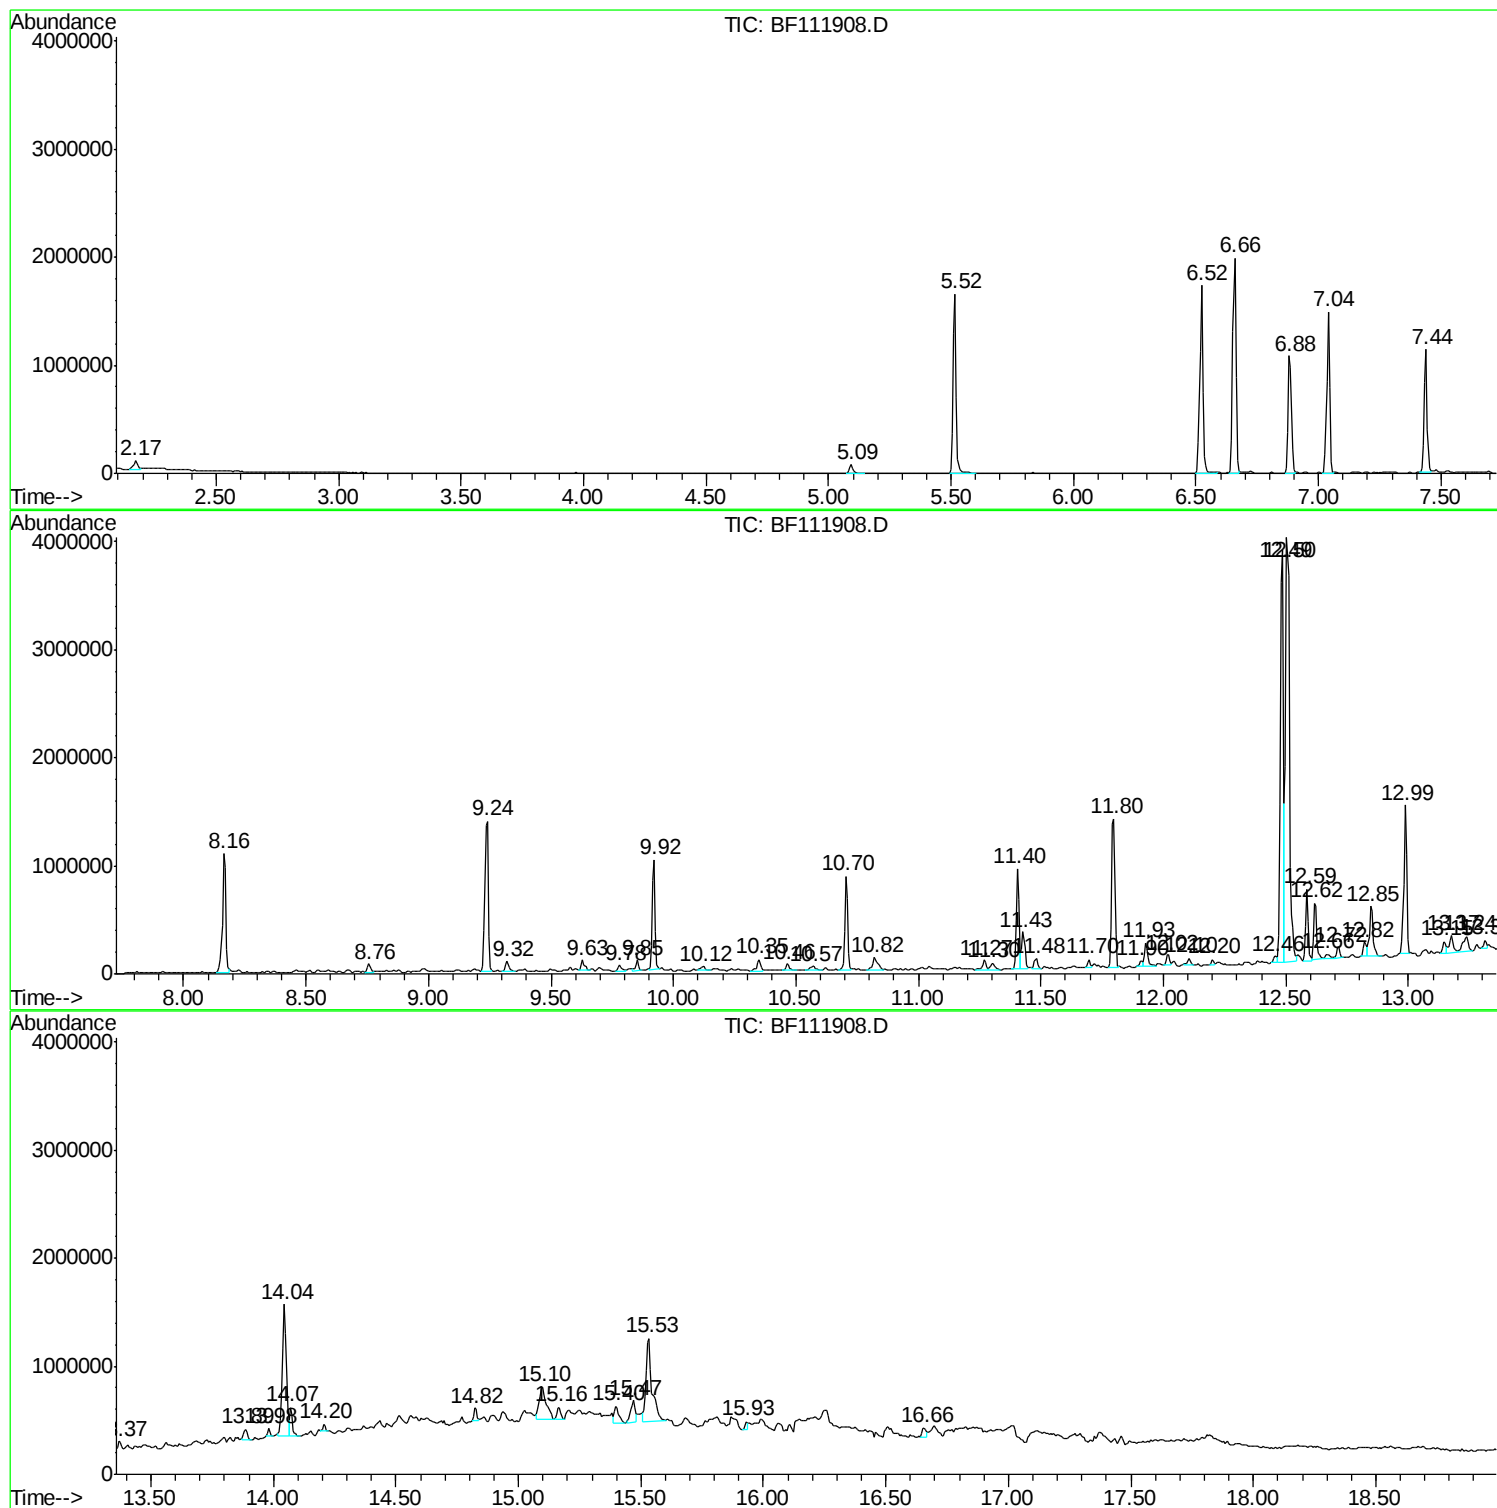

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010819\
Data_File : BF111908.D
Acq_On : 8-Jan-2019 15:477
Operator : JU/SJJ
Sample : K1012-05RE_2XX
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
EO-02-010419-CRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
