


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010819\
 Data File : BF111904.D
 Acq On : 8 Jan 2019 13:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 07 14:33:51 2019

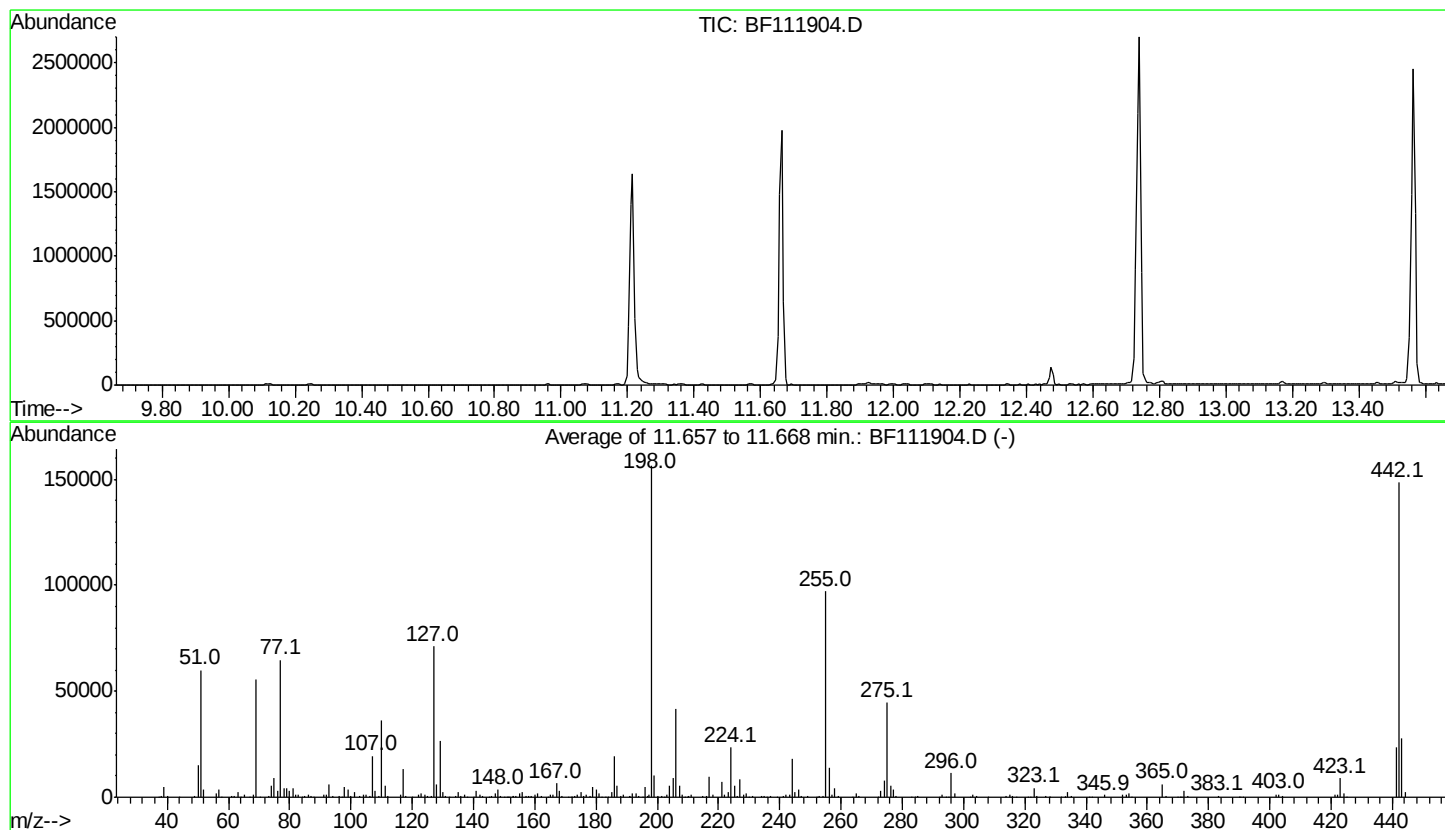

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	60003	PASS
68	69	0.00	2	1.8	1013	PASS
69	198	0.00	100	35.4	55392	PASS
70	69	0.00	2	0.4	234	PASS
127	198	10	80	45.5	71120	PASS
197	198	0.00	2	0.7	1135	PASS
198	198	100	100	100.0	156466	PASS
199	198	5	9	6.5	10225	PASS
275	198	10	60	28.5	44570	PASS
365	198	1	100	3.9	6070	PASS
441	198	0.01	100	15.2	23861	PASS
442	198	50	100	94.9	148560	PASS
443	442	15	24	18.8	27912	PASS