


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010819\
 Data File : BF111931.D
 Acq On : 9 Jan 2019 2:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 07 14:33:51 2019

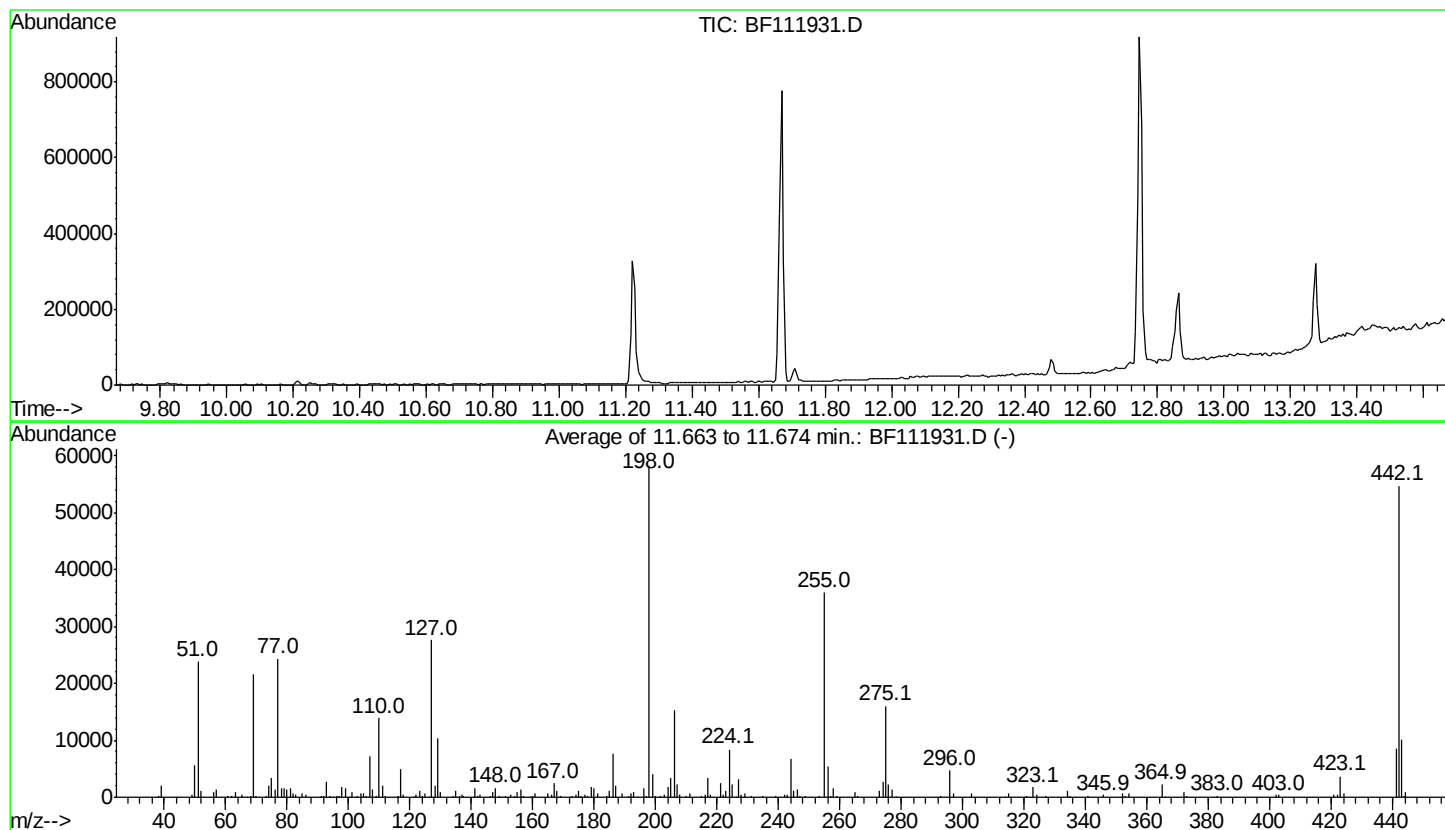

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	23721	PASS
68	69	0.00	2	1.2	266	PASS
69	198	0.00	100	37.2	21650	PASS
70	69	0.00	2	1.0	217	PASS
127	198	10	80	47.4	27598	PASS
197	198	0.00	2	0.5	295	PASS
198	198	100	100	100.0	58218	PASS
199	198	5	9	7.1	4154	PASS
275	198	10	60	27.5	16011	PASS
365	198	1	100	3.8	2241	PASS
441	198	0.01	100	14.7	8546	PASS
442	198	50	100	93.9	54650	PASS
443	442	15	24	18.4	10080	PASS