
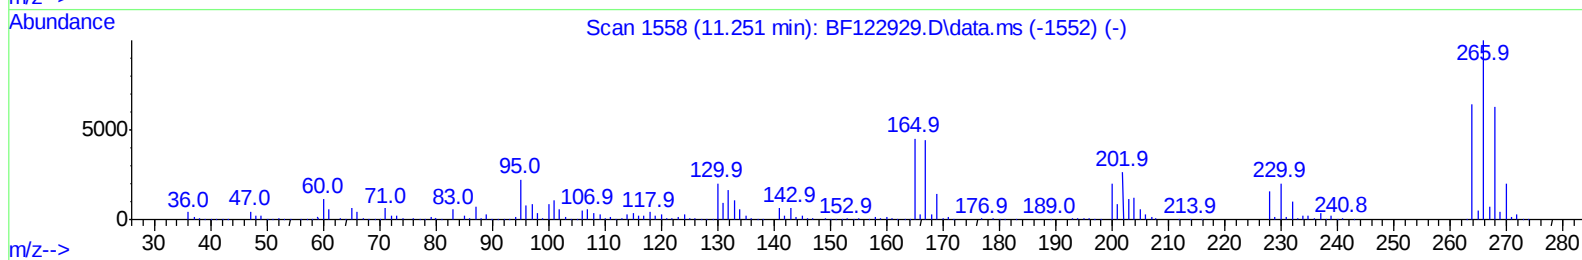
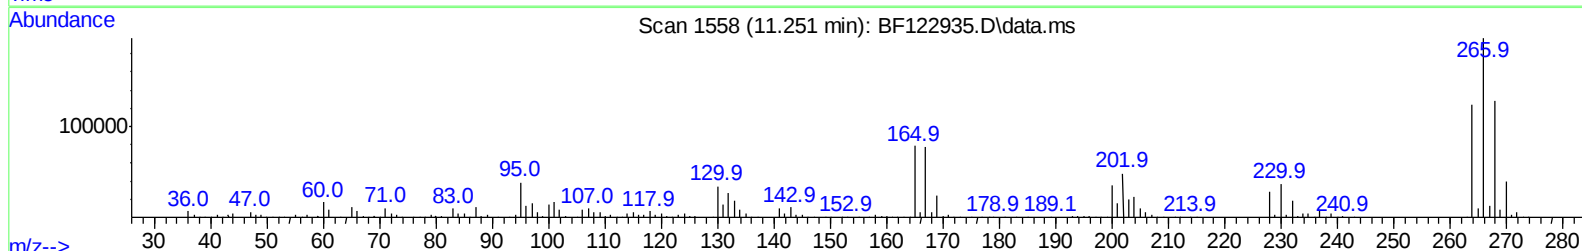


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010821\
Data File : BF122935.D
Acq On : 8 Jan 2021 11:49
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 02:28:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 08 16:17:19 2021
Response via : Initial Calibration

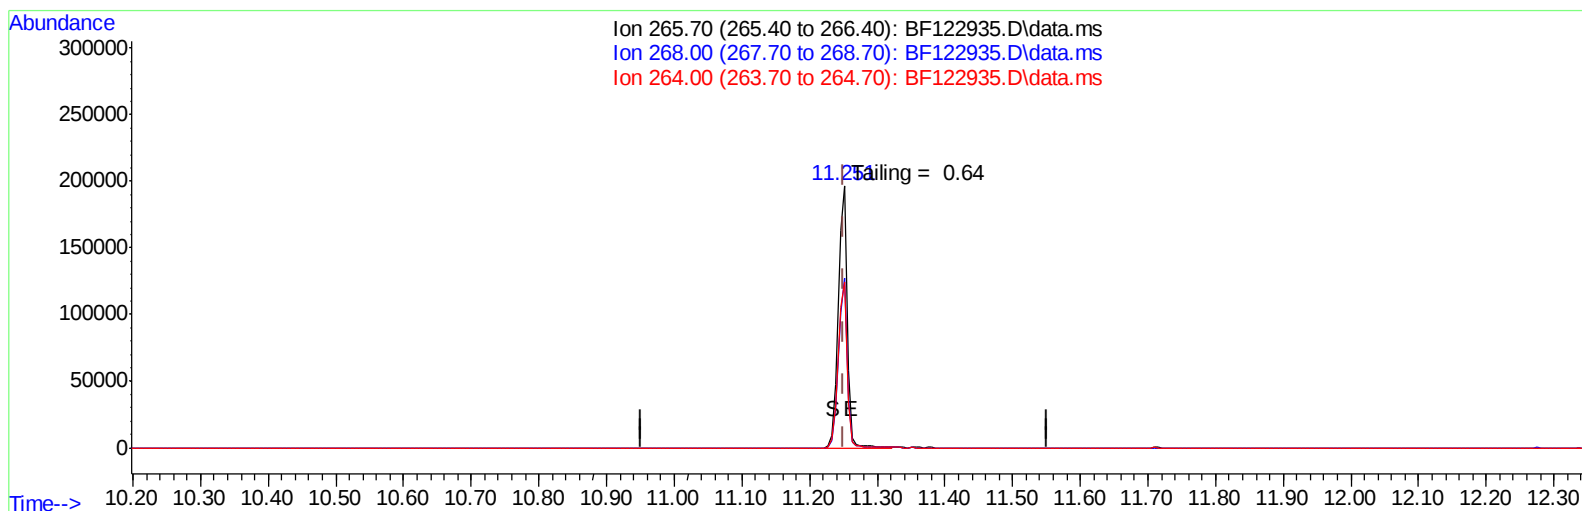

TIC: BF122935.D\data.ms

(70) Pentachlorophenol (C)




11.251min (-0.000) 20578.92 ng

response 175333

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.78
264.00	62.30	63.26
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010821\  
Data File : BF122935.D  
Acq On    : 8 Jan 2021 11:49  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Jan 09 02:28:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 08 16:17:19 2021
Response via : Initial Calibration

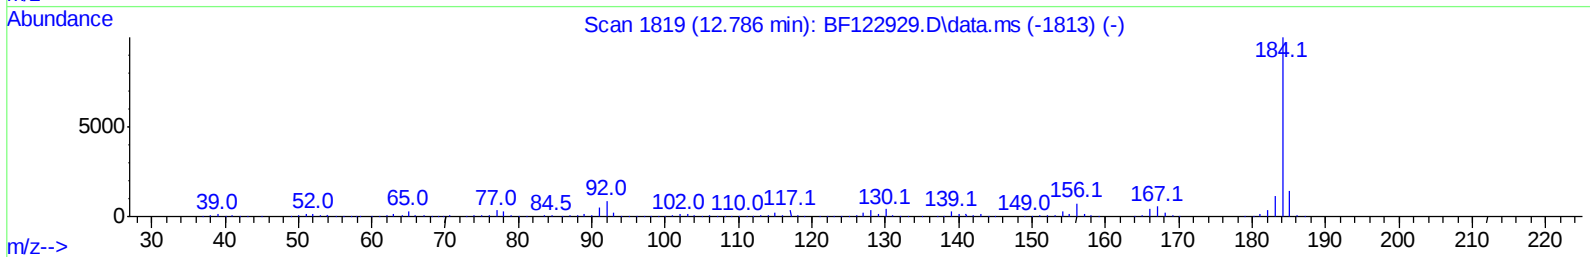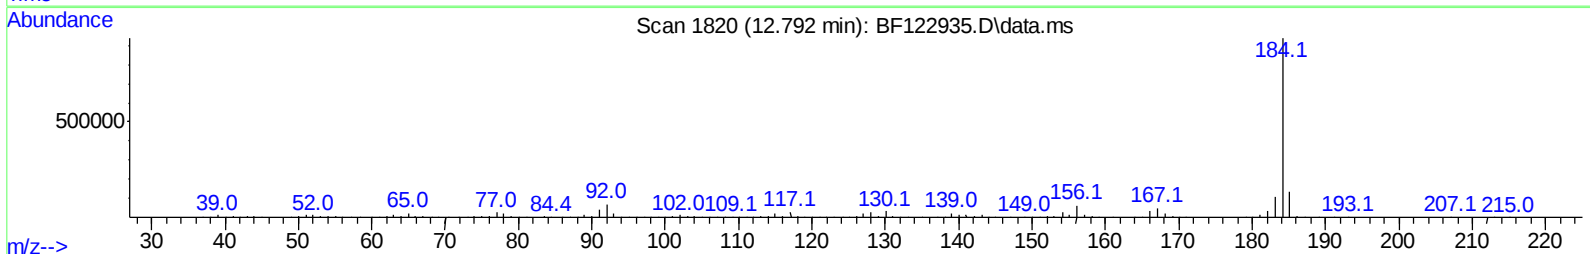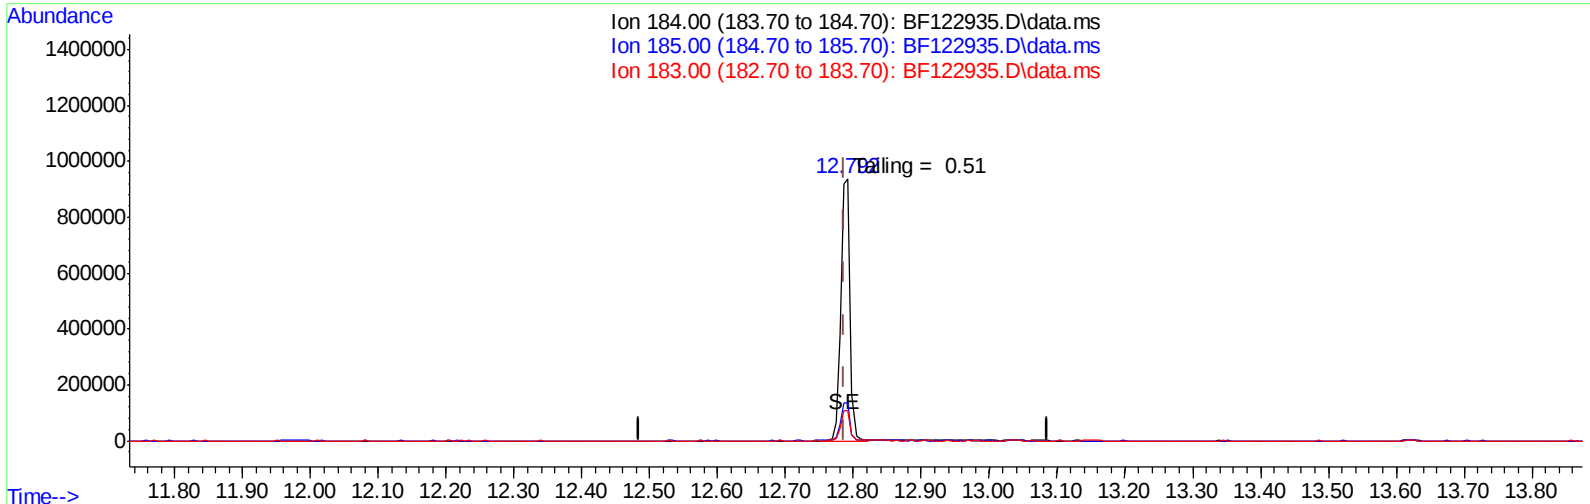

TIC: BF122935.D\data.ms

(77) Benzidine

12.792min (+ 0.006) 15148.95 ng

response **888831**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.19
183.00	12.10	11.47
0.00	0.00	0.00