

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010821\
 Data File : BF122947.D
 Acq On : 8 Jan 2021 18:32
 Operator : JU/CG
 Sample : M1044-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

mohammad
 1/11/2021 10:27:29 AM

Quant Time: Jan 08 23:31:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 08 16:17:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.916	152	175010	20.00	ng	0.00
21) Naphthalene-d8	8.198	136	642285	20.00	ng	0.00
39) Acenaphthene-d10	9.957	164	321605	20.00	ng	0.00
64) Phenanthrene-d10	11.445	188	534348	20.00	ng	0.00
76) Chrysene-d12	14.098	240	424137	20.00	ng	0.00
86) Perylene-d12	15.592	264	477889	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.534	112	1225067	105.09	ng	0.00
7) Phenol-d6	6.534	99	1511424	95.54	ng	0.00
23) Nitrobenzene-d5	7.475	82	888878	68.43	ng	0.00
42) 2,4,6-Tribromophenol	10.745	330	366491	100.89	ng	-0.01
45) 2-Fluorobiphenyl	9.275	172	1541582	67.95	ng	0.00
79) Terphenyl-d14	13.045	244	1336011	58.36	ng	0.00
Target Compounds						Qvalue
10) Phenol	6.540	94	33566	2.14	ng	80
50) Dimethylphthalate	9.669	163	102253	4.27	ng	100
71) Phenanthrene	11.469	178	174016	5.75	ng	98
75) Fluoranthene	12.663	202	339849	10.55	ng	99
78) Pyrene	12.892	202	324852	9.85	ng	98
81) Benzo(a)anthracene	14.086	228	191025	6.71	ng	99
83) Chrysene	14.121	228	159295	5.81	ng	97
88) Benzo(b)fluoranthene	15.151	252	233055m	6.94	ng	
89) Benzo(k)fluoranthene	15.180	252	77873m	2.52	ng	
90) Benzo(a)pyrene	15.521	252	179697	6.09	ng	# 91
92) Benzo(g,h,i)perylene	17.545	276	103378	4.29	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010821\
Data File : BF122947.D
Acq On : 8 Jan 2021 18:32
Operator : JU/CG
Sample : M1044-03
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
TP-4

Manual Integrations
APPROVED

mohammad
1/11/2021 10:27:29 AM


Quant Time: Jan 08 23:31:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 08 16:17:19 2021
Response via : Initial Calibration

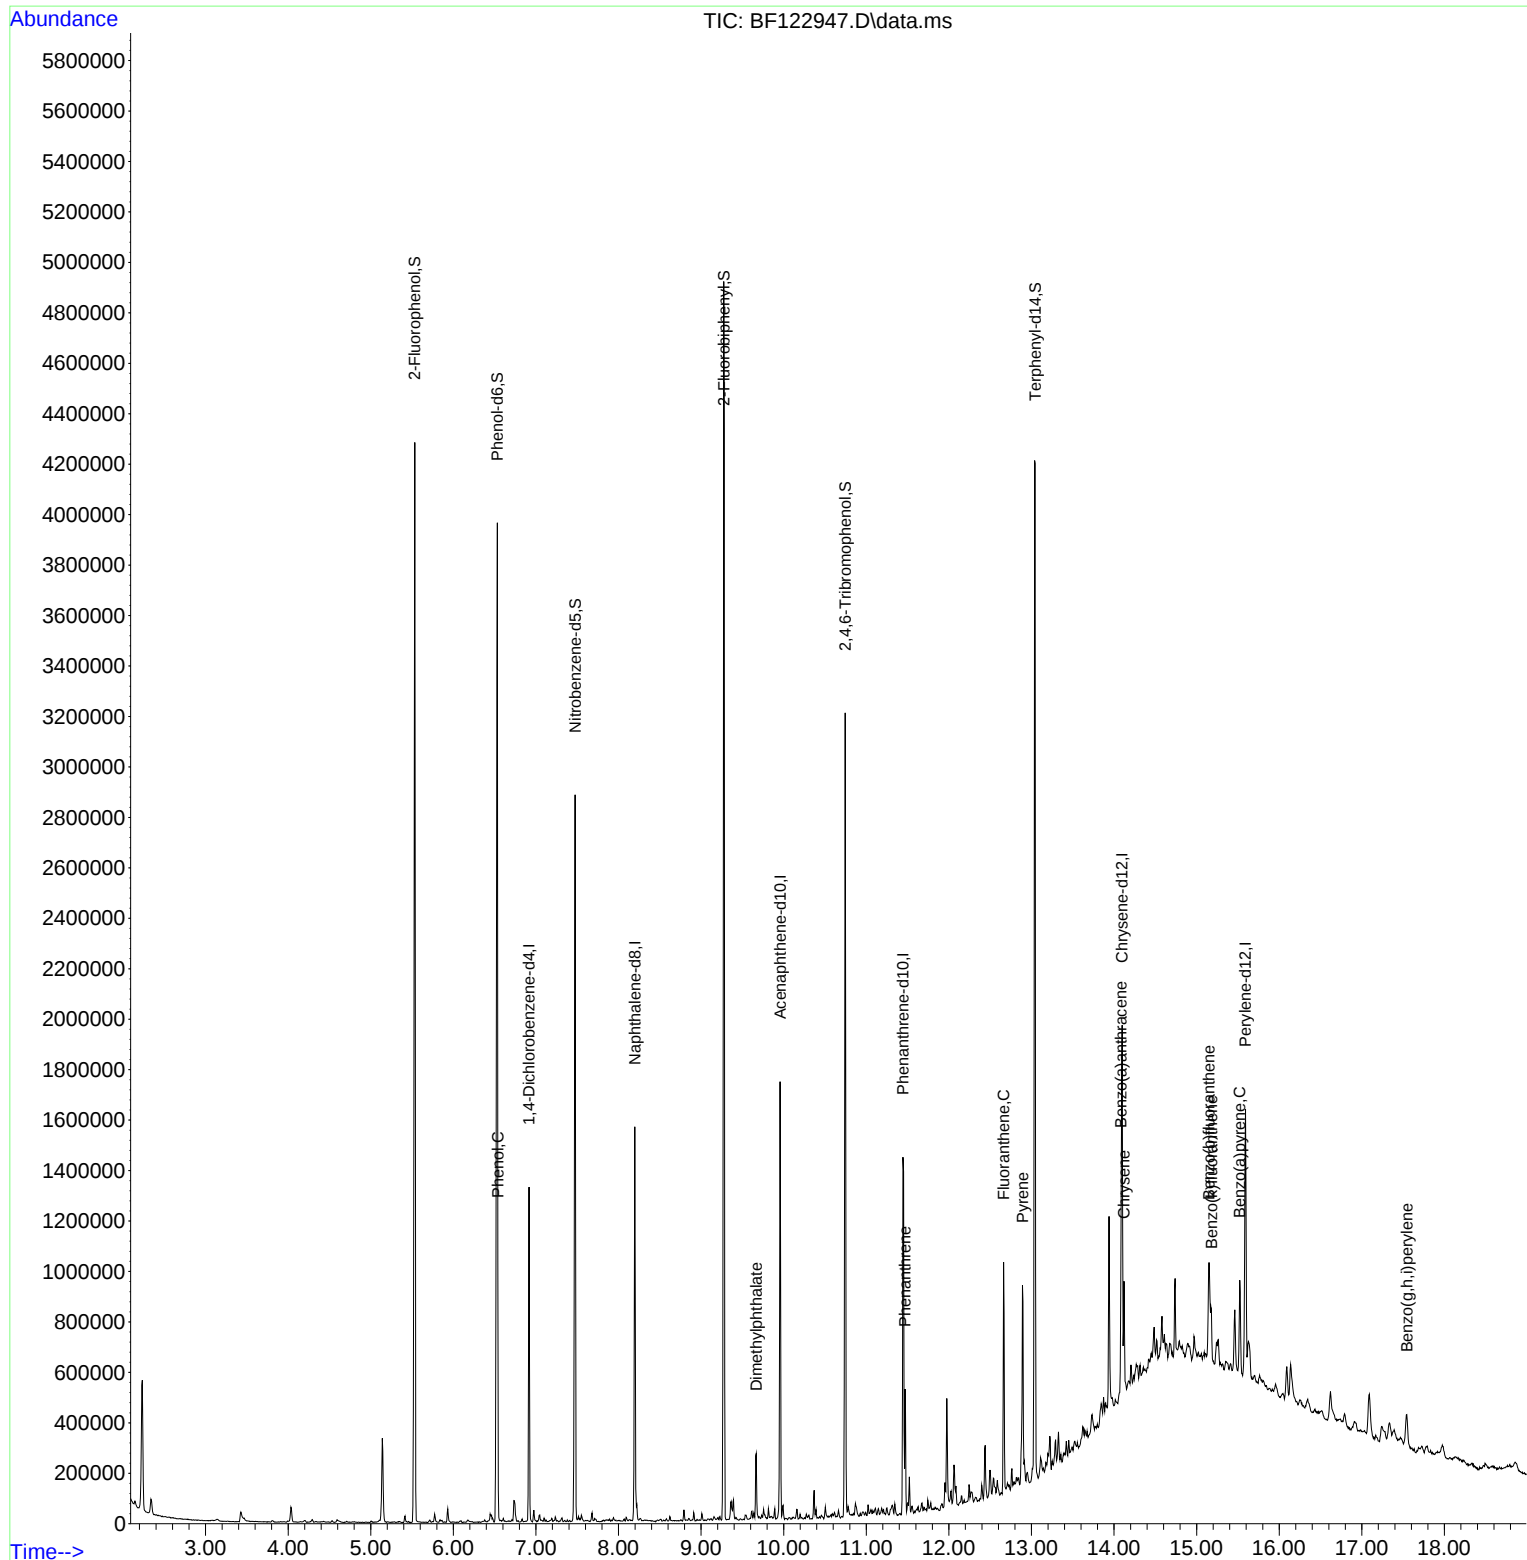



#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.916 min Scan# 821
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Instrument :
BNA_F
ClientSampleId :
TP-4




Tgt Ion:152 Resp: 175010
Ion Ratio Lower Upper
152 100
150 155.2 125.8 188.6
115 57.8 49.3 73.9

Manual Integrations
APPROVED



mohammad
1/11/2021 10:27:29 AM

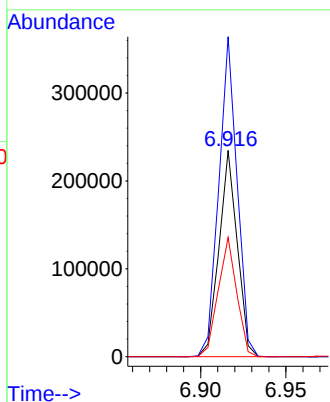


#5
2-Fluorophenol
Concen: 105.09 ng
RT: 5.534 min Scan# 586
Delta R.T. -0.000 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Tgt Ion:112 Resp: 1225067
Ion Ratio Lower Upper
112 100
64 57.8 46.9 70.3
63 29.1 24.5 36.7

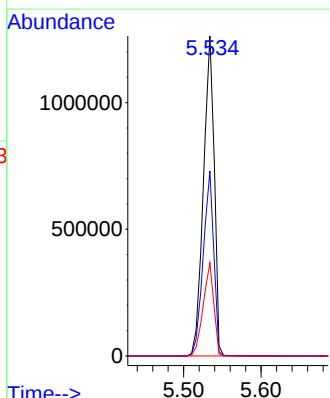



#7
Phenol-d6
Concen: 95.54 ng
RT: 6.534 min Scan# 756
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

Instrument :
BNA_F
ClientSampled :
TP-4






Tgt Ion: 99 Resp: 1511424


Ion	Ratio	Lower	Upper
99	100		
42	15.6	13.8	20.6
71	30.8	26.9	40.3

Manual Integrations
APPROVED

mohammad
1/11/2021 10:27:29 AM

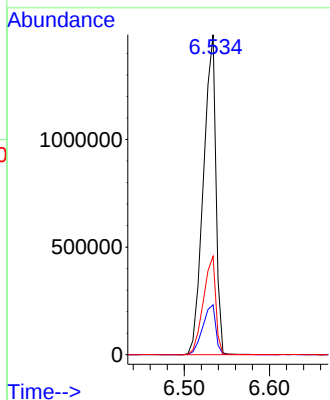




#10
Phenol
Concen: 2.14 ng
RT: 6.540 min Scan# 757
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32



Tgt Ion: 94 Resp: 33566


Ion	Ratio	Lower	Upper
94	100		
65	35.7	11.2	51.2
66	63.8	25.8	65.8

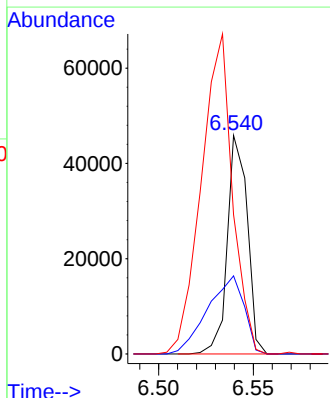



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.198 min Scan# 1039
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

Instrument :
BNA_F
ClientSampled :
TP-4






Tgt Ion:136 Resp: 642285


Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.8	13.2
54	7.8	5.5	8.3
68	6.7	4.6	6.8

Manual Integrations
APPROVED

mohammad
1/11/2021 10:27:29 AM

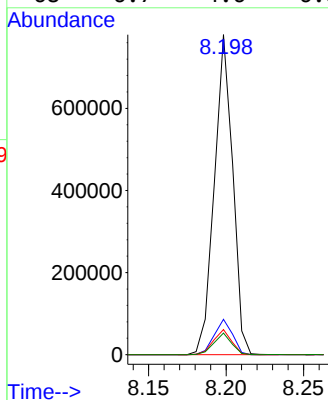
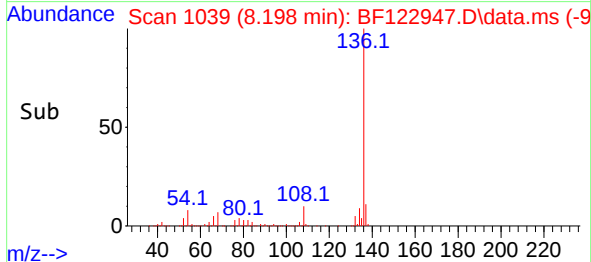



#23
Nitrobenzene-d5
Concen: 68.43 ng
RT: 7.475 min Scan# 916
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Tgt Ion: 82 Resp: 888878

Ion	Ratio	Lower	Upper
82	100		
128	46.1	37.0	55.4
54	46.7	38.4	57.6


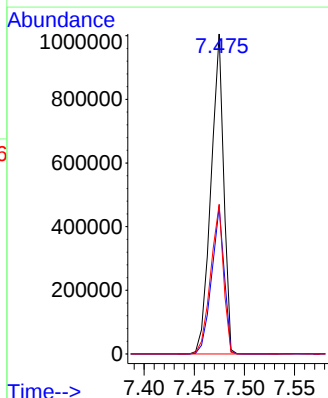






#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.957 min Scan# 1338
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32





Tgt Ion:164 Resp: 321605
Ion Ratio Lower Upper
164 100
162 99.2 80.8 121.2
160 44.0 35.4 53.0

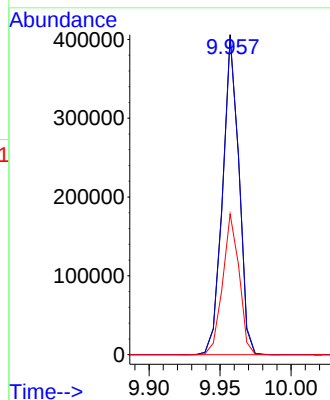

#42
2,4,6-Tribromophenol
Concen: 100.89 ng
RT: 10.745 min Scan# 1472
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

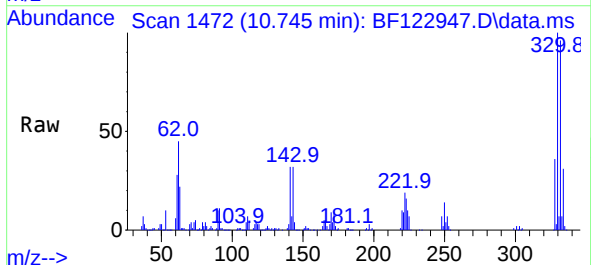


Tgt Ion:330 Resp: 366491
Ion Ratio Lower Upper
330 100
332 95.8 77.5 116.3
141 31.5 23.8 35.8

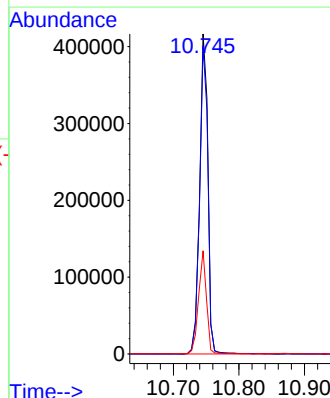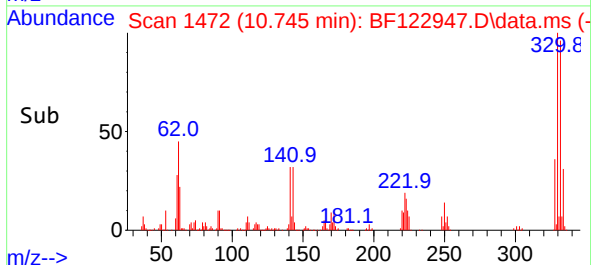

Instrument :
BNA_F
ClientSampleId :
TP-4


Manual Integrations
APPROVED

mohammad
1/11/2021 10:27:29 AM



#45
2-Fluorobiphenyl
Concen: 67.95 ng
RT: 9.275 min Scan# 1222
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Instrument :
BNA_F
ClientSampled :
TP-4




Tgt Ion:172 Resp: 1541582
Ion Ratio Lower Upper
172 100
171 37.1 29.6 44.4
170 24.9 19.5 29.3

Manual Integrations
APPROVED



mohammad
1/11/2021 10:27:29 AM

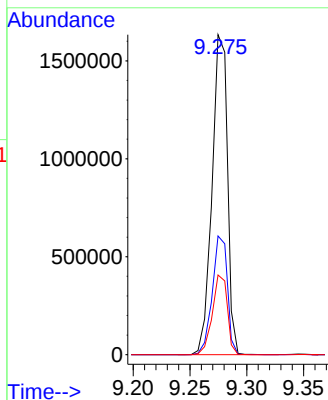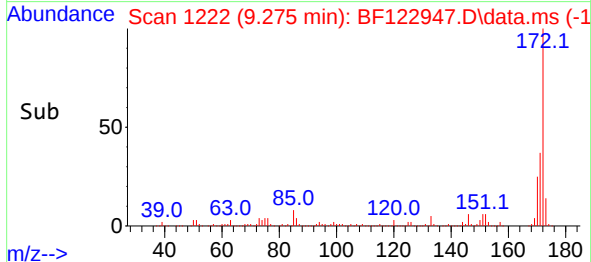


#50
Dimethylphthalate
Concen: 4.27 ng
RT: 9.669 min Scan# 1289
Delta R.T. -0.018 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Tgt Ion:163 Resp: 102253
Ion Ratio Lower Upper
163 100
194 4.5 3.4 5.0
164 10.0 8.1 12.1

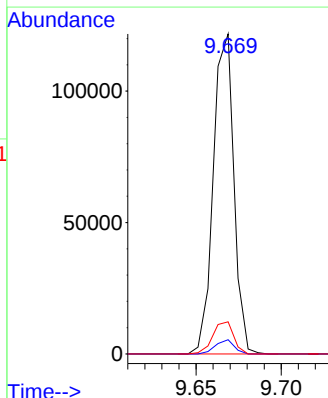



#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.445 min Scan# 1591
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Instrument :
BNA_F
ClientSampled :
TP-4




Tgt Ion:188 Resp: 534348
Ion Ratio Lower Upper
188 100
94 10.5 7.4 11.2
80 11.4 8.2 12.4

Manual Integrations
APPROVED



mohammad
1/11/2021 10:27:29 AM

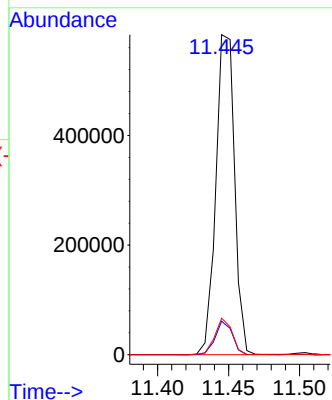


#71
Phenanthrene
Concen: 5.75 ng
RT: 11.469 min Scan# 1595
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Tgt Ion:178 Resp: 174016
Ion Ratio Lower Upper
178 100
176 19.1 16.2 24.2
179 14.8 12.7 19.1

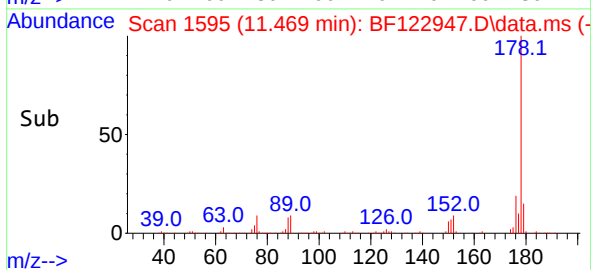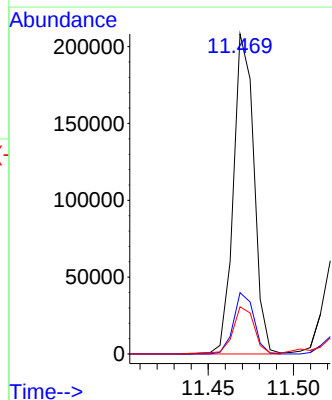



#75
Fluoranthene
Concen: 10.55 ng
RT: 12.663 min Scan# 1798
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Instrument :
BNA_F
ClientSampled :
TP-4




Tgt Ion:202 Resp: 339849
Ion Ratio Lower Upper
202 100
101 12.6 0.0 32.2
203 17.6 0.0 38.1

Manual Integrations
APPROVED



mohammad
1/11/2021 10:27:29 AM

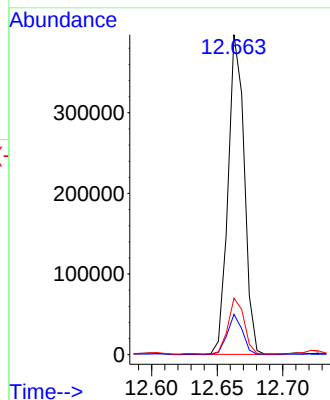


#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.098 min Scan# 2042
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32



Tgt Ion:240 Resp: 424137
Ion Ratio Lower Upper
240 100
120 10.7 8.6 12.8
236 26.3 20.3 30.5

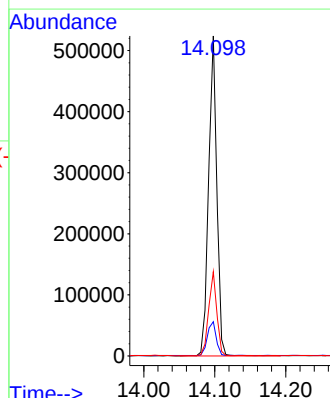







#78
Pyrene
Concen: 9.85 ng
RT: 12.892 min Scan# 1837
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

Tgt Ion:202 Resp: 324852
Ion Ratio Lower Upper
202 100
200 20.7 17.6 26.4
203 18.5 14.6 21.8

Instrument :
BNA_F
ClientSampleId :
TP-4




Manual Integrations
APPROVED


mohammad
1/11/2021 10:27:29 AM

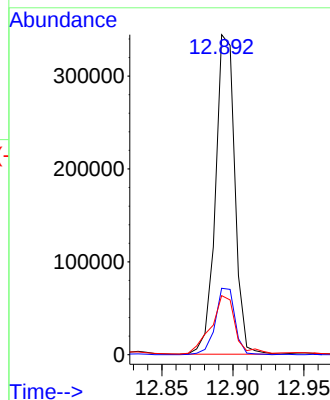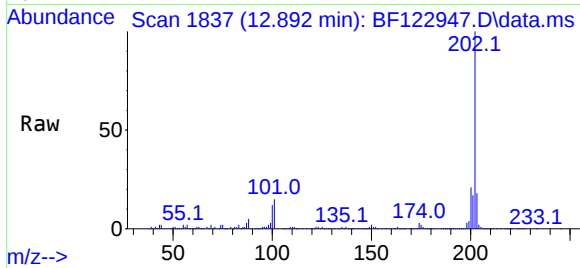


#79
Terphenyl-d14
Concen: 58.36 ng
RT: 13.045 min Scan# 1863
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

Tgt Ion:244 Resp: 1336011
Ion Ratio Lower Upper
244 100
212 7.3 5.7 8.5
122 10.1 8.3 12.5

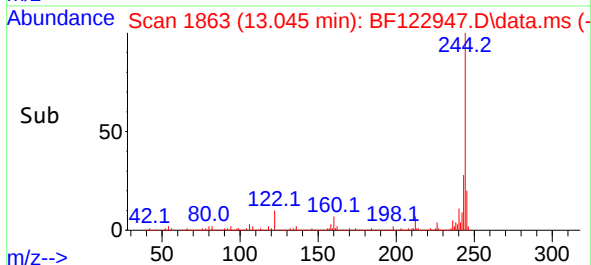
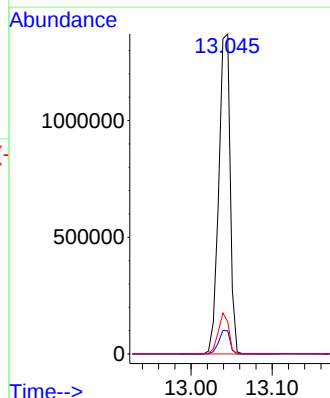
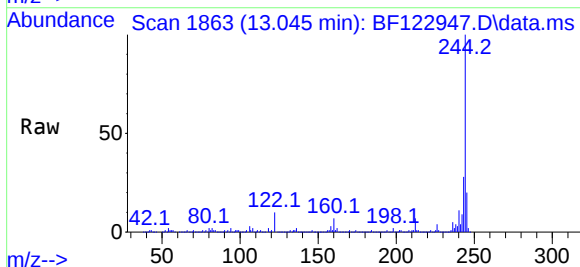





#81
Benzo(a)anthracene
Concen: 6.71 ng
RT: 14.086 min Scan# 2040
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32





Tgt Ion:228 Resp: 191025
Ion Ratio Lower Upper
228 100
226 29.6 23.0 34.4
229 21.0 16.6 24.8

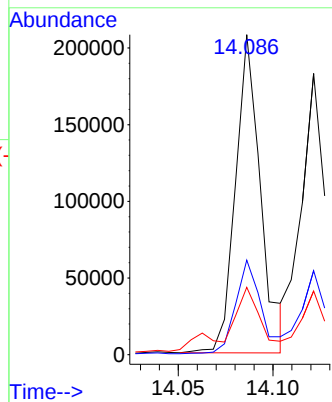

#83
Chrysene
Concen: 5.81 ng
RT: 14.121 min Scan# 2046
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

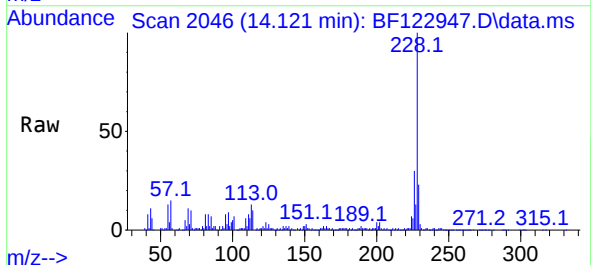


Tgt Ion:228 Resp: 159295
Ion Ratio Lower Upper
228 100
226 29.9 24.6 36.8
229 22.6 15.8 23.6

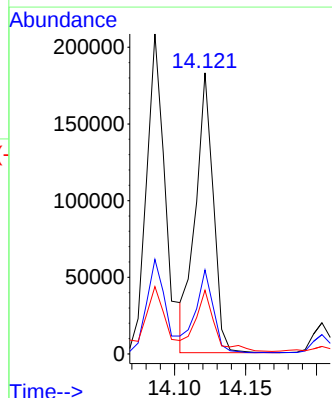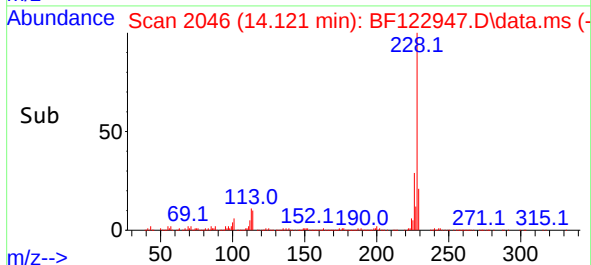

Instrument :
BNA_F
ClientSampled :
TP-4


Manual Integrations
APPROVED

mohammad
1/11/2021 10:27:29 AM



#86
Perylene-d12
Concen: 20.00 ng
RT: 15.592 min Scan# 2296
Delta R.T. 0.000 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

Instrument :
BNA_F
ClientSampled :
TP-4






Tgt Ion:264 Resp: 477889


Ion	Ratio	Lower	Upper
264	100		
260	24.3	18.6	28.0
265	22.0	17.0	25.6

Manual Integrations
APPROVED

mohammad
1/11/2021 10:27:29 AM

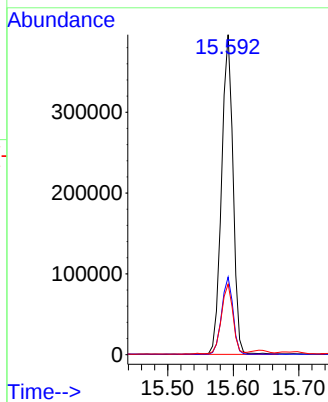
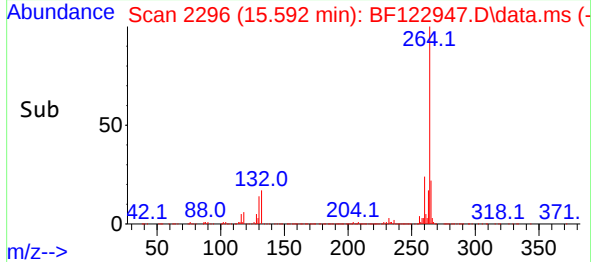



#88
Benzo(b)fluoranthene
Concen: 6.94 ng m
RT: 15.151 min Scan# 2221
Delta R.T. -0.006 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

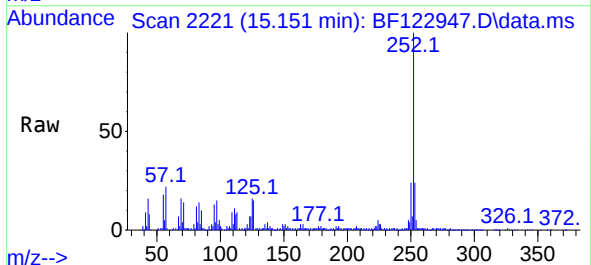

Tgt Ion:252 Resp: 233055


Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.3	27.5
125	15.8	8.1	12.1

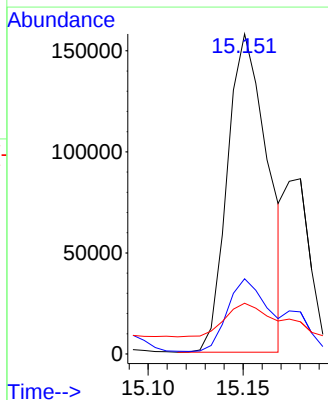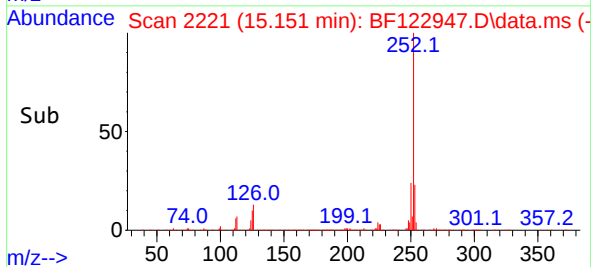



#89
Benzo(k)fluoranthene
Concen: 2.52 ng m
RT: 15.180 min Scan# 2226
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32




Instrument :
BNA_F
ClientSampled :
TP-4

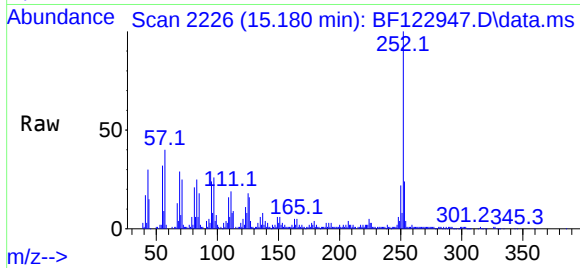


Tgt Ion:252 Resp: 77873
Ion Ratio Lower Upper
252 100
253 24.1 17.8 26.8
125 18.4 8.4 12.6#

Manual Integrations
APPROVED



mohammad
1/11/2021 10:27:29 AM

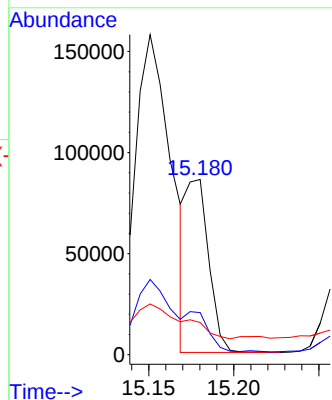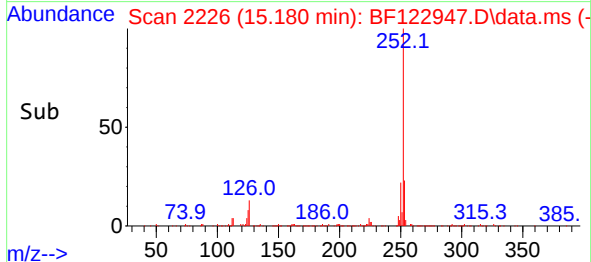


#90
Benzo(a)pyrene
Concen: 6.09 ng
RT: 15.521 min Scan# 2284
Delta R.T. -0.012 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32

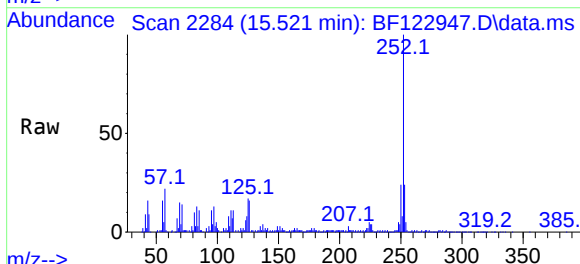


Tgt Ion:252 Resp: 179697
Ion Ratio Lower Upper
252 100
253 24.3 17.5 26.3
125 16.6 8.6 12.8#

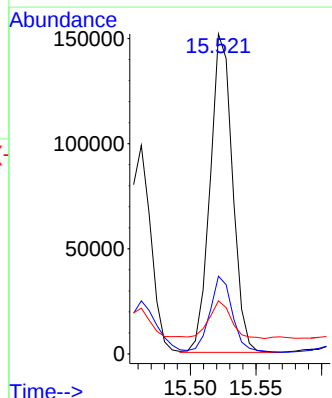





#92
Benzo(g,h,i)perylene
Concen: 4.29 ng
RT: 17.545 min Scan# 2628
Delta R.T. -0.018 min
Lab File: BF122947.D
Acq: 8 Jan 2021 18:32



Tgt Ion: 276 Resp: 103378
Ion Ratio Lower Upper
276 100
277 24.8 19.3 28.9
138 23.0 16.6 24.8

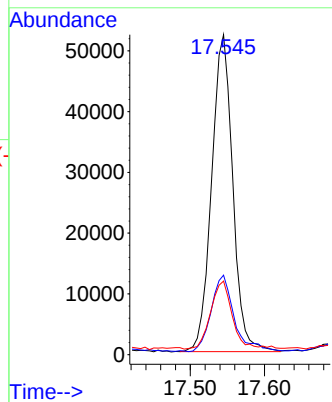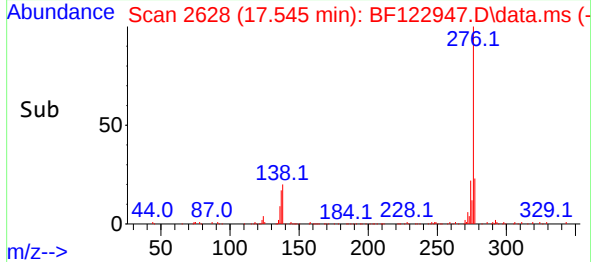

Instrument :
BNA_F
ClientSampleId :
TP-4

Manual Integrations
APPROVED

mohammad
1/11/2021 10:27:29 AM