
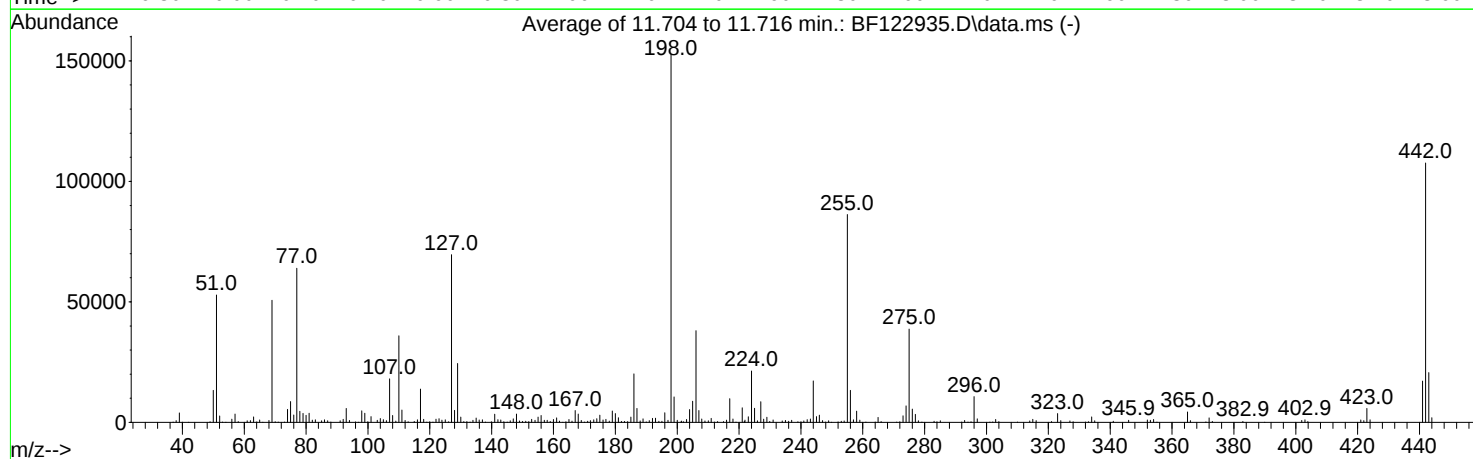


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010821\
 Data File : BF122935.D
 Acq On : 8 Jan 2021 11:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 08 16:17:19 2021

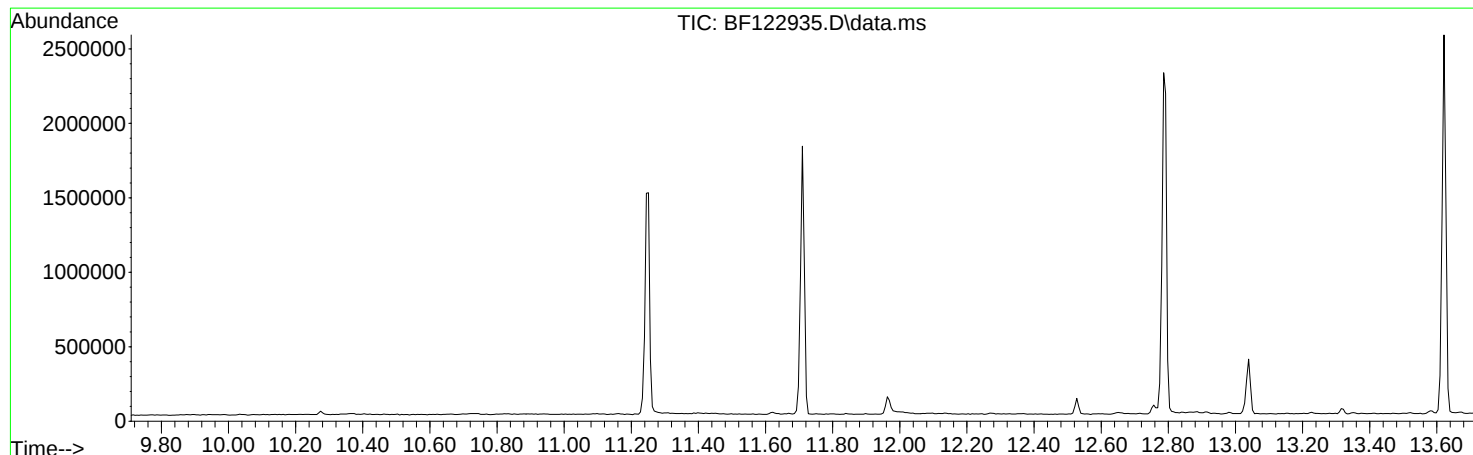

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	52837	PASS
68	69	0.00	2	1.6	796	PASS
69	198	0.00	100	33.2	50641	PASS
70	69	0.00	2	0.5	276	PASS
127	198	10	80	45.6	69595	PASS
197	198	0.00	2	0.6	858	PASS
198	198	100	100	100.0	152651	PASS
199	198	5	9	6.9	10578	PASS
275	198	10	60	25.4	38728	PASS
365	198	1	100	2.8	4310	PASS
441	198	0.01	100	11.2	17155	PASS
442	198	50	100	70.5	107611	PASS
443	442	15	24	19.2	20636	PASS