
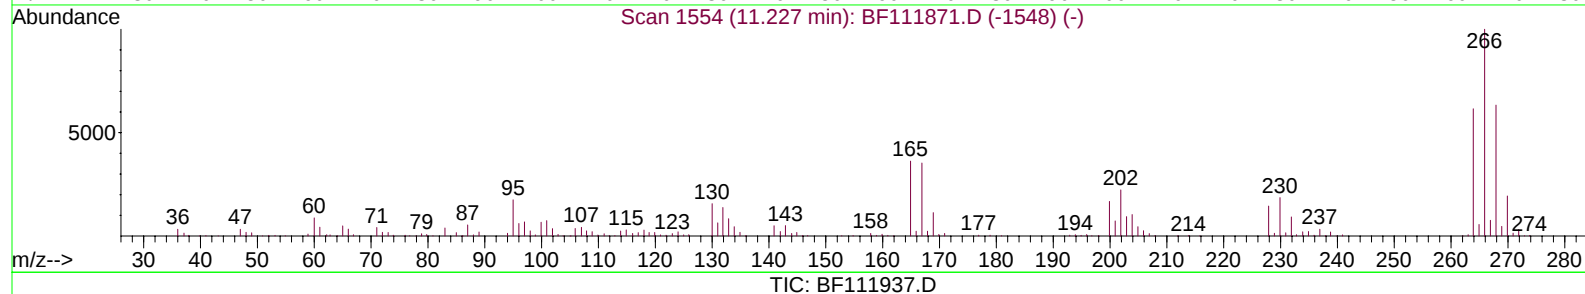
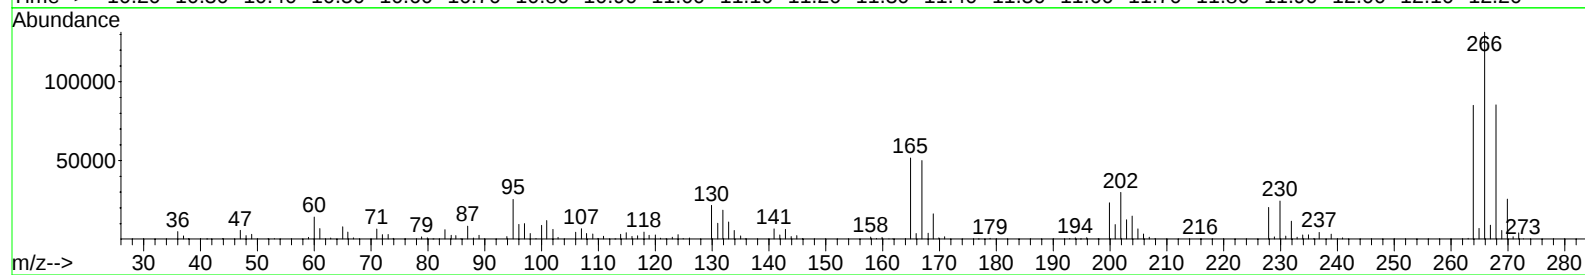


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010919\
Data File : BF111937.D
Acq On : 9 Jan 2019 8:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 11:34:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 07 14:33:51 2019
Response via : Initial Calibration

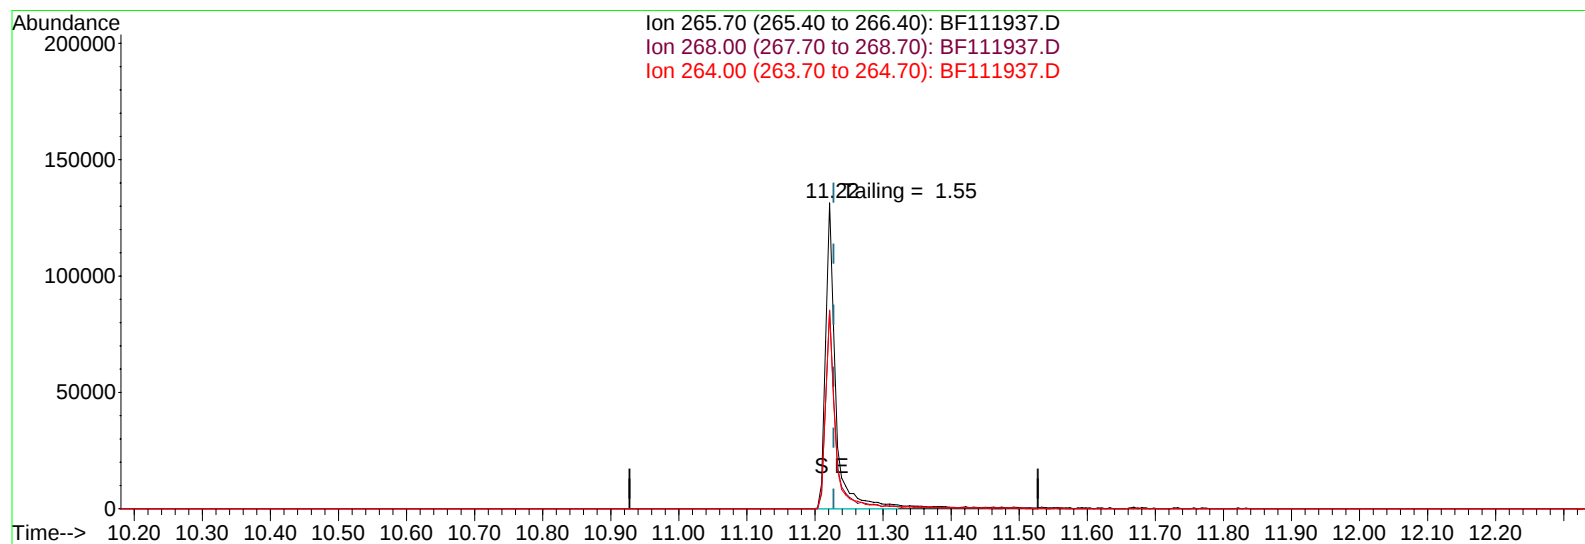

(70) Pentachlorophenol (C)




11.221min (-0.006) 31063.04ng m

response 135241

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	64.94
264.00	61.60	64.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010919\
Data File : BF111937.D
Acq On : 9 Jan 2019 8:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 11:34:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 07 14:33:51 2019
Response via : Initial Calibration

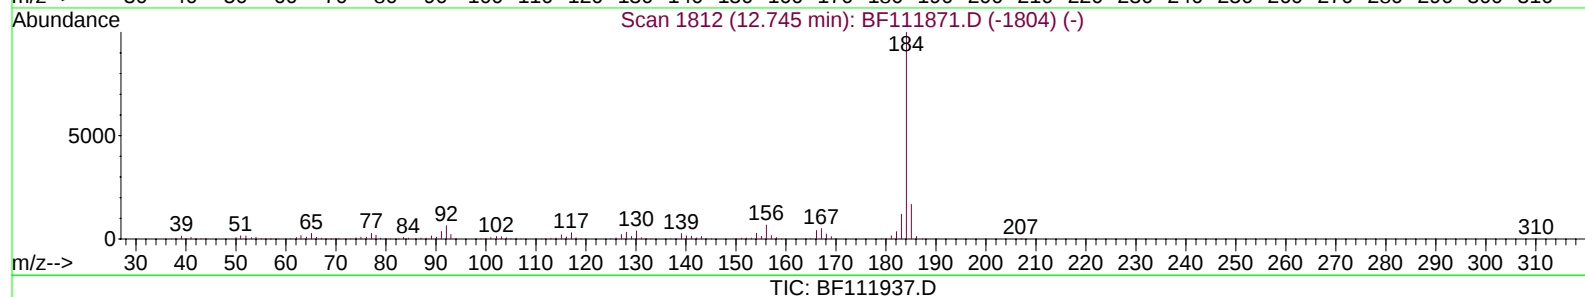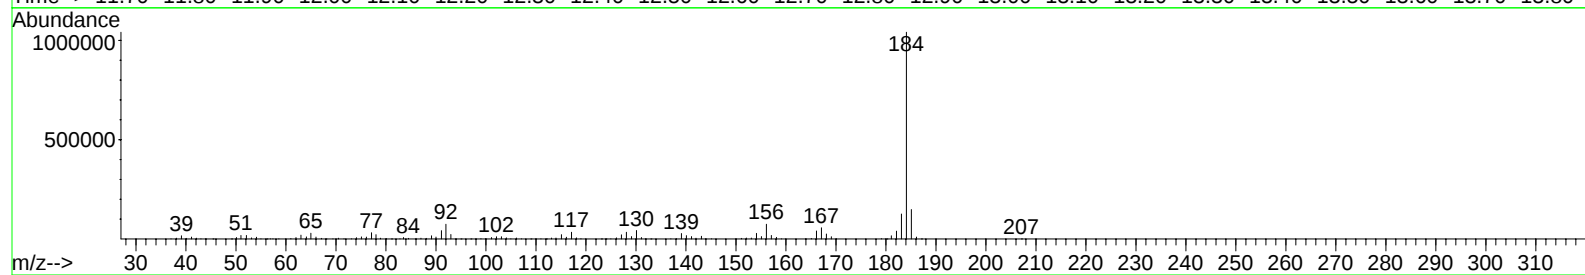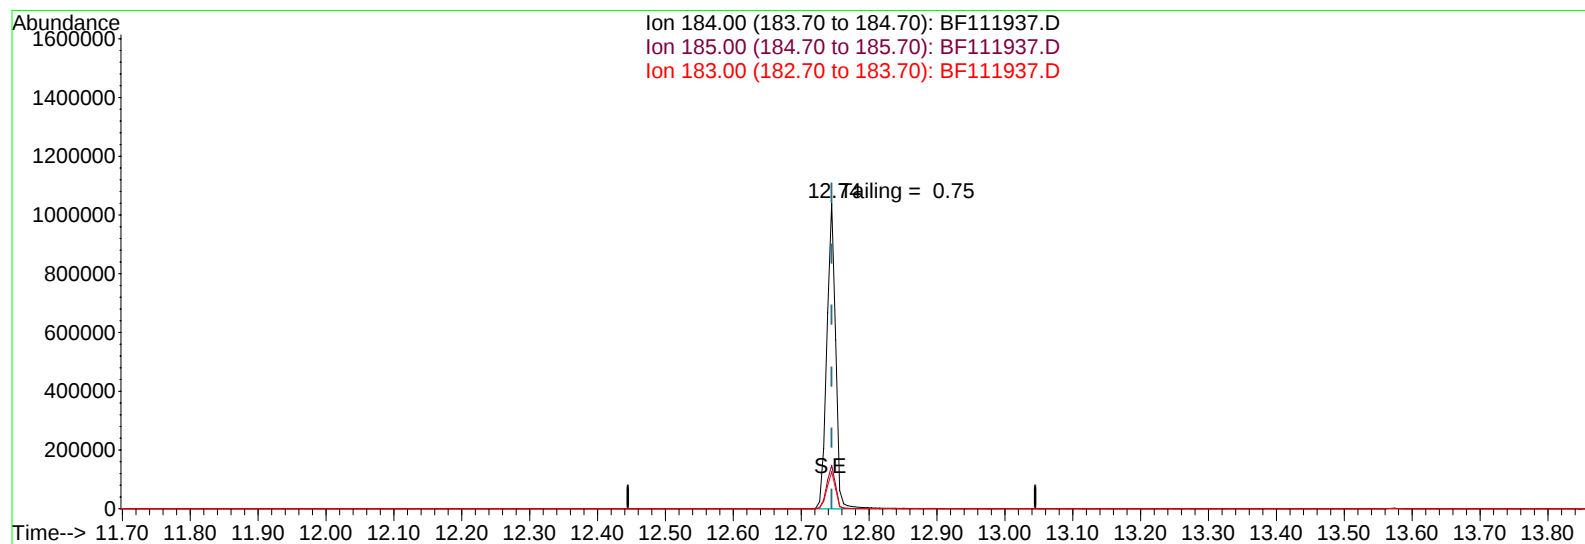

(77) Benzidine

12.745min (-0.000) 0.00ng

response 934912

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.24
183.00	12.00	12.08
0.00	0.00	0.00