
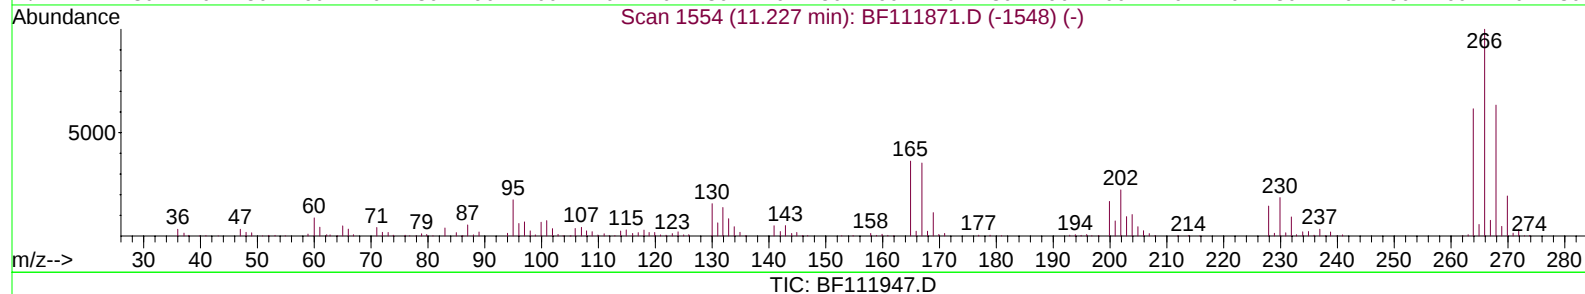
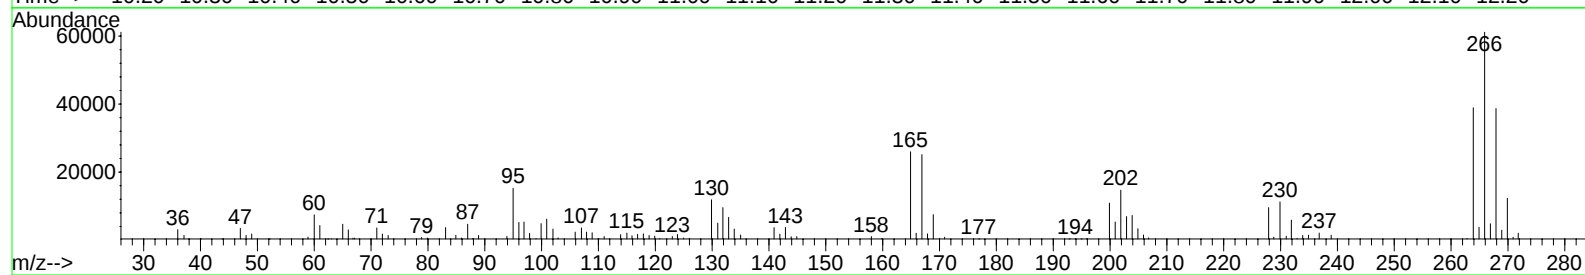


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010919\
Data File : BF111947.D
Acq On : 9 Jan 2019 13:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 16:22:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 07 14:33:51 2019
Response via : Initial Calibration

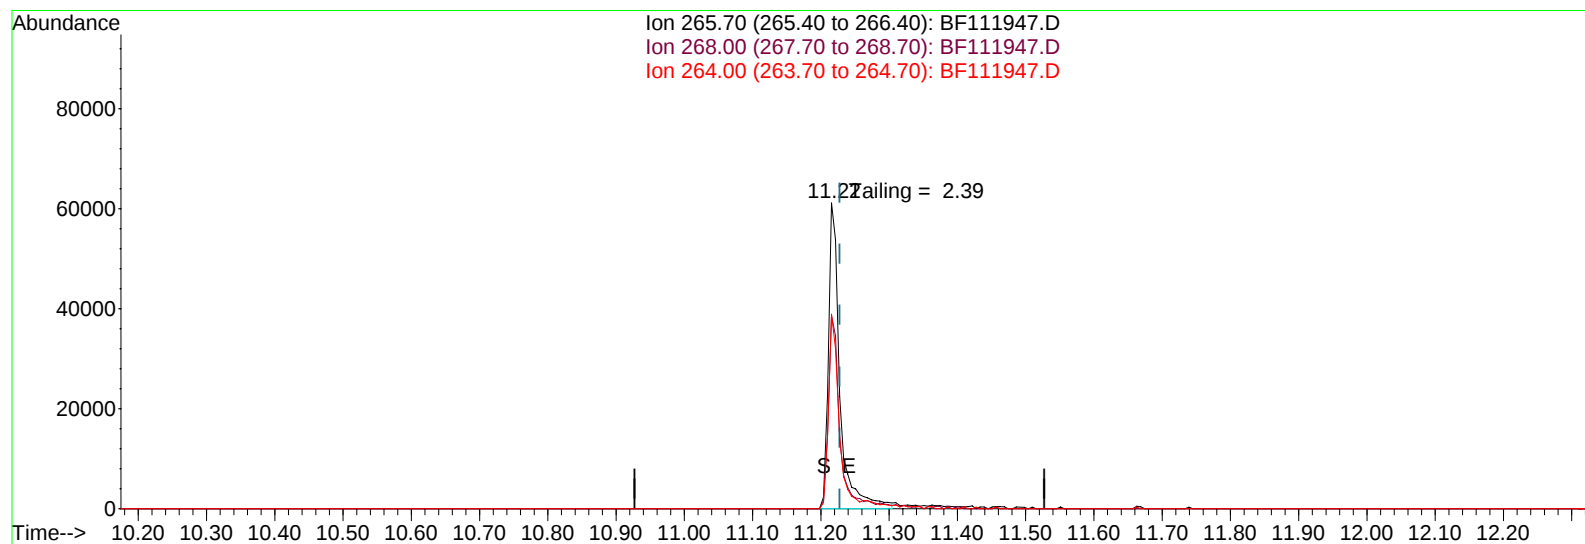

(70) Pentachlorophenol (C)




11.216min (-0.012) 27576.62ng

response 72758

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	63.27
264.00	61.60	63.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010919\
 Data File : BF111947.D
 Acq On : 9 Jan 2019 13:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 16:22:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 07 14:33:51 2019
 Response via : Initial Calibration

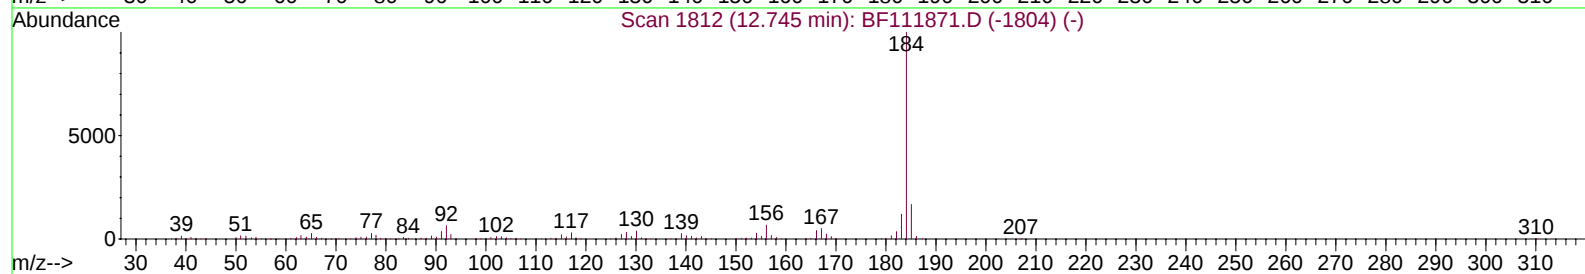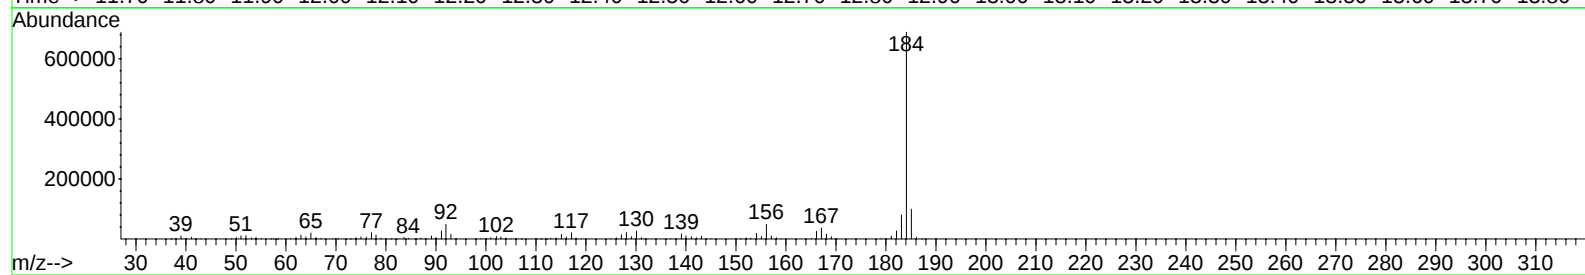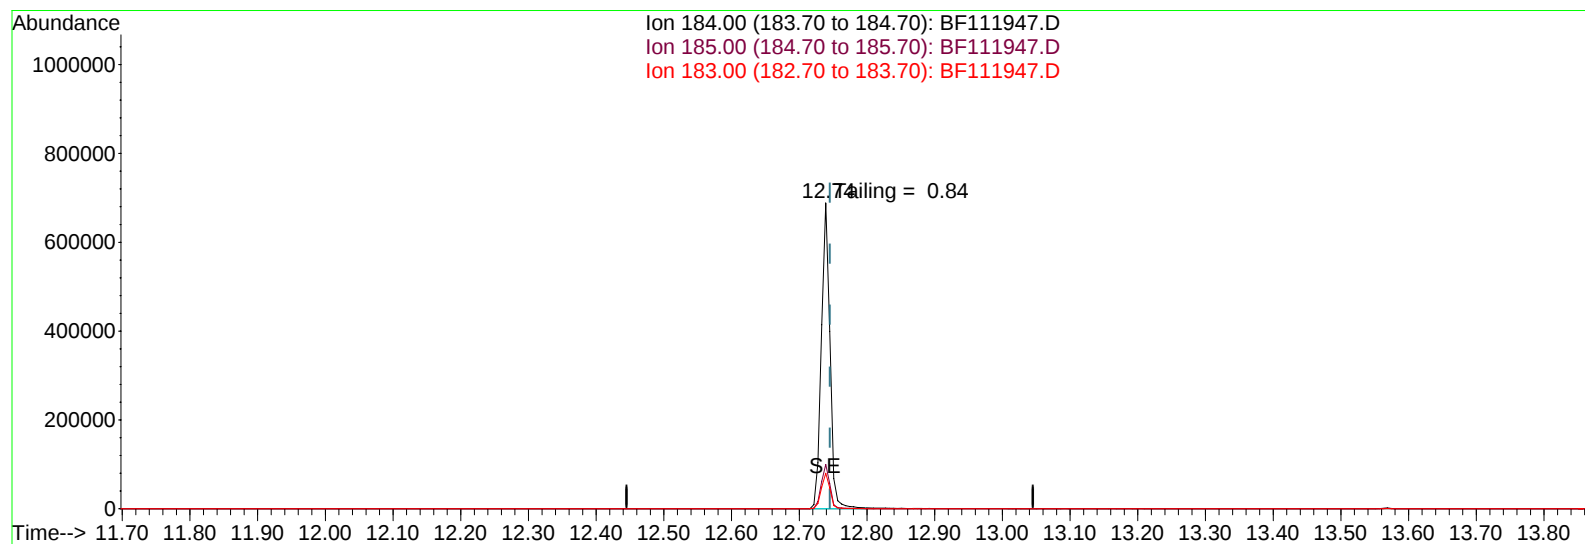

TIC: BF111947.D

(77) Benzidine

12.739min (-0.006) 0.00ng

response 617185

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.48
183.00	12.00	11.64
0.00	0.00	0.00