


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010919\
 Data File : BF111937.D
 Acq On : 9 Jan 2019 8:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 07 14:33:51 2019

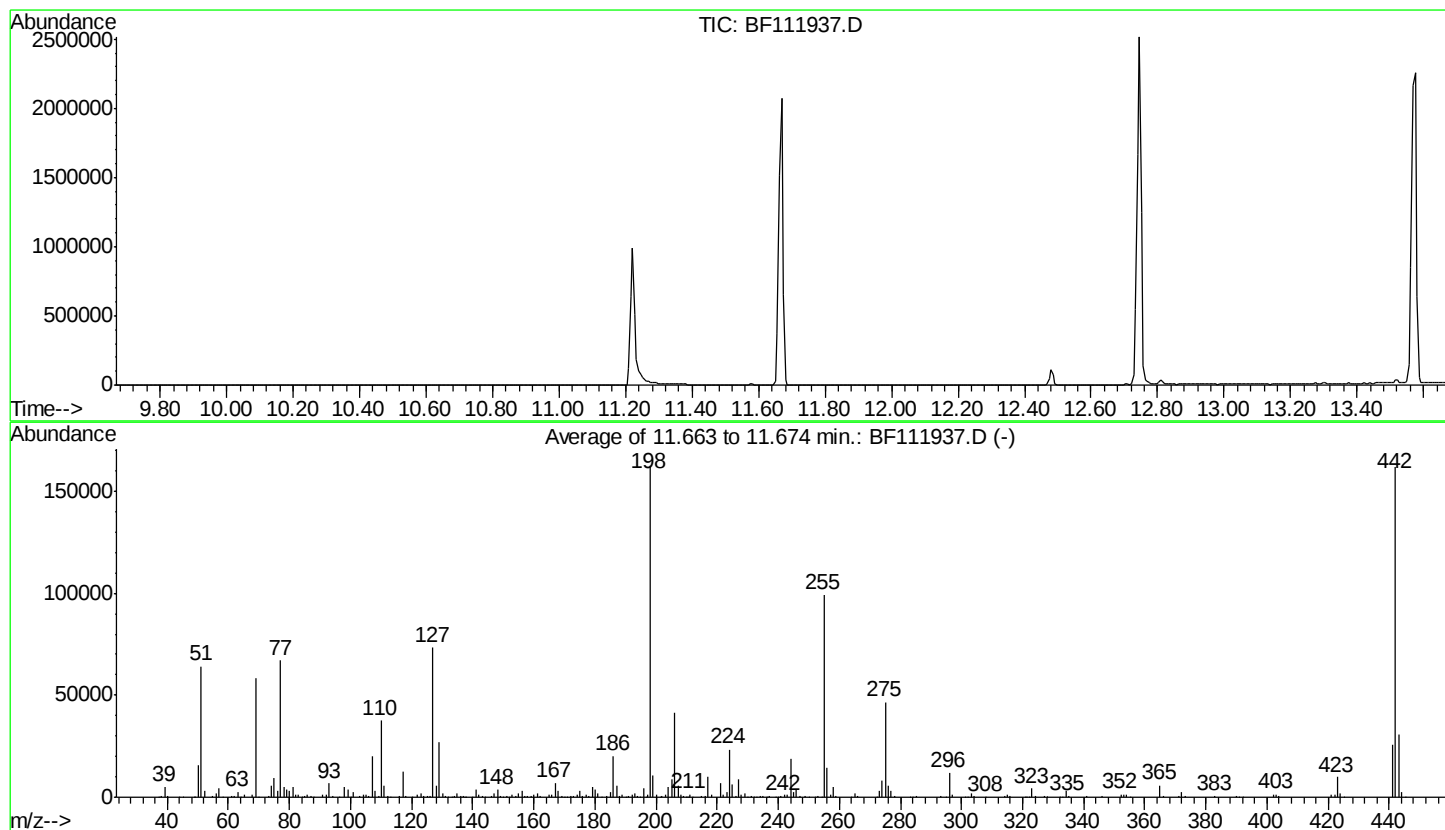

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	64186	PASS
68	69	0.00	2	2.0	1153	PASS
69	198	0.00	100	35.9	58419	PASS
70	69	0.00	2	0.4	259	PASS
127	198	10	80	45.0	73149	PASS
197	198	0.00	2	0.6	1020	PASS
198	198	100	100	100.0	162528	PASS
199	198	5	9	6.4	10439	PASS
275	198	10	60	28.7	46677	PASS
365	198	1	100	3.6	5870	PASS
441	198	0.01	100	15.8	25605	PASS
442	198	50	100	99.5	161778	PASS
443	442	15	24	19.0	30714	PASS