


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011019\
 Data File : BF111981.D
 Acq On : 10 Jan 2019 11:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 07 14:33:51 2019

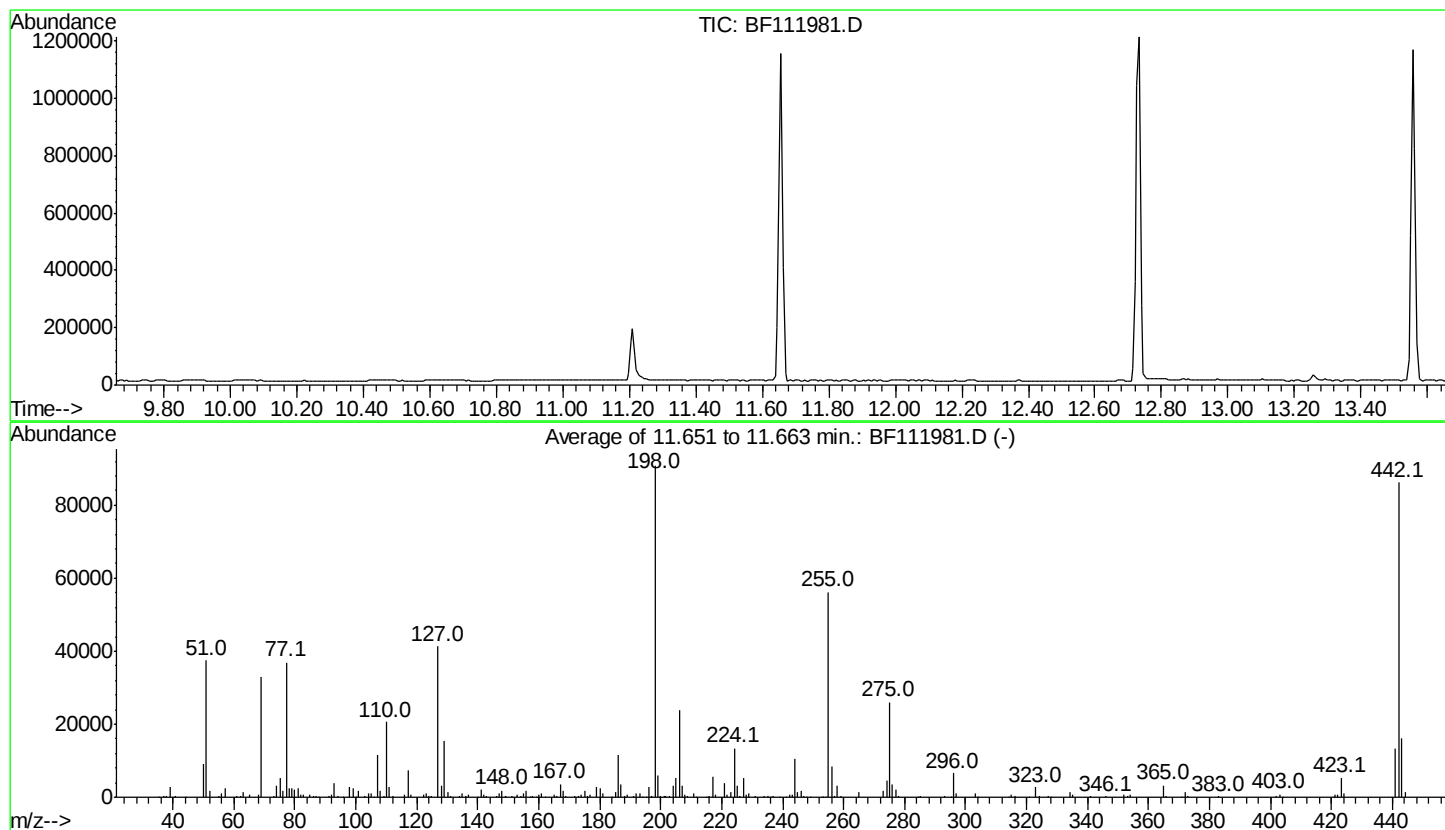

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	37380	PASS
68	69	0.00	2	2.0	650	PASS
69	198	0.00	100	36.3	32992	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.4	41252	PASS
197	198	0.00	2	0.4	351	PASS
198	198	100	100	100.0	90810	PASS
199	198	5	9	6.4	5853	PASS
275	198	10	60	28.6	25966	PASS
365	198	1	100	3.6	3298	PASS
441	198	0.01	100	14.5	13193	PASS
442	198	50	100	94.9	86173	PASS
443	442	15	24	18.9	16299	PASS