
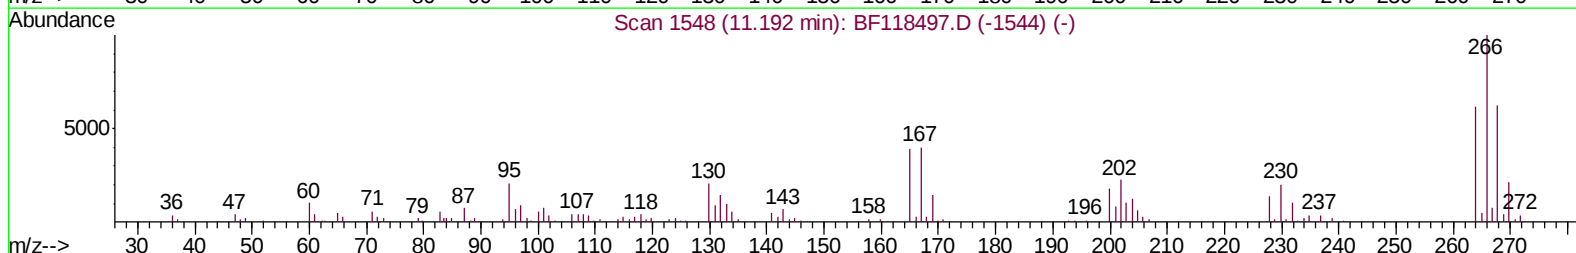
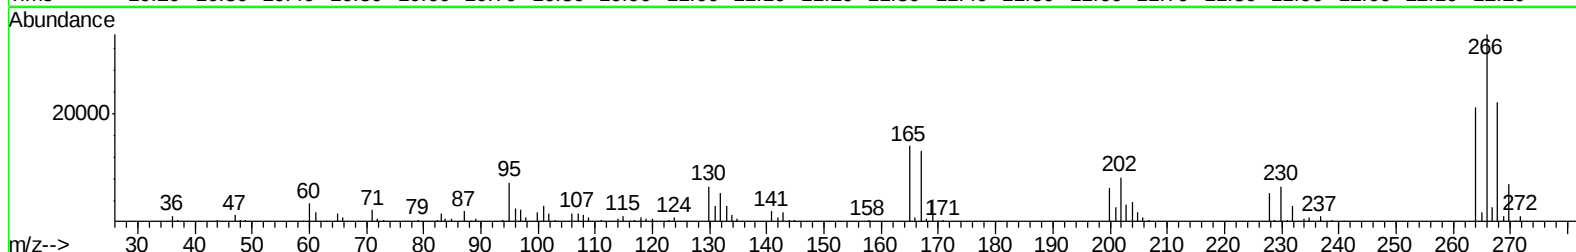


Data File : BF118513.D
Acq On : 10 Jan 2020 11:45
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 03:45:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 16:06:11 2020
Response via : Initial Calibration

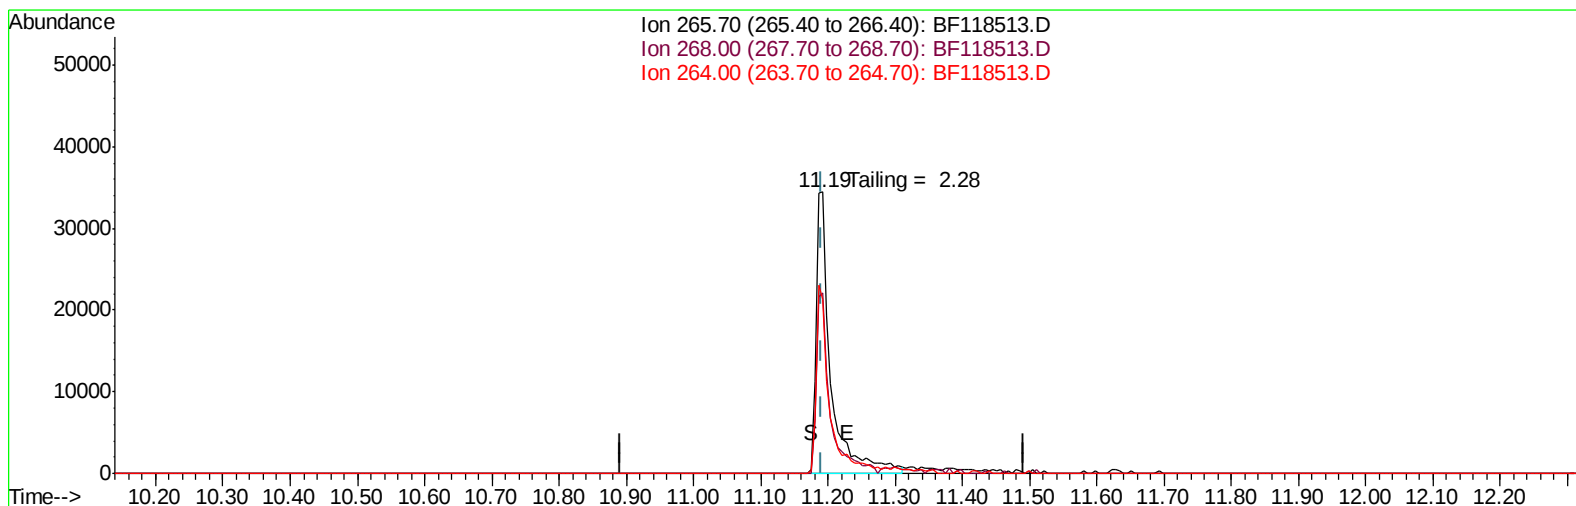

TIC: BF118513.D

(70) Pentachlorophenol (C)




11.192min (+0.000) 37697.49ng

response 53319

Ion	Exp%	Act%
265.70	100	100
268.00	62.70	64.25
264.00	61.70	61.65
0.00	0.00	0.00

Data File : BF118513.D
Acq On : 10 Jan 2020 11:45
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 03:45:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 16:06:11 2020
Response via : Initial Calibration

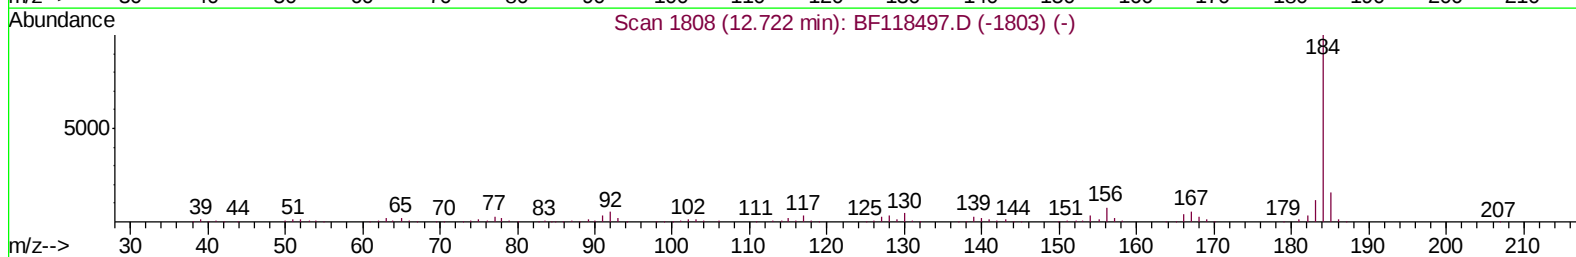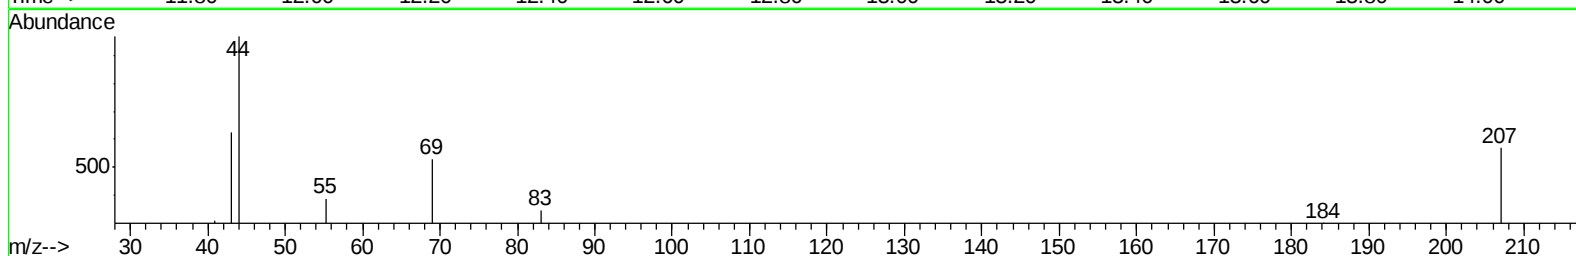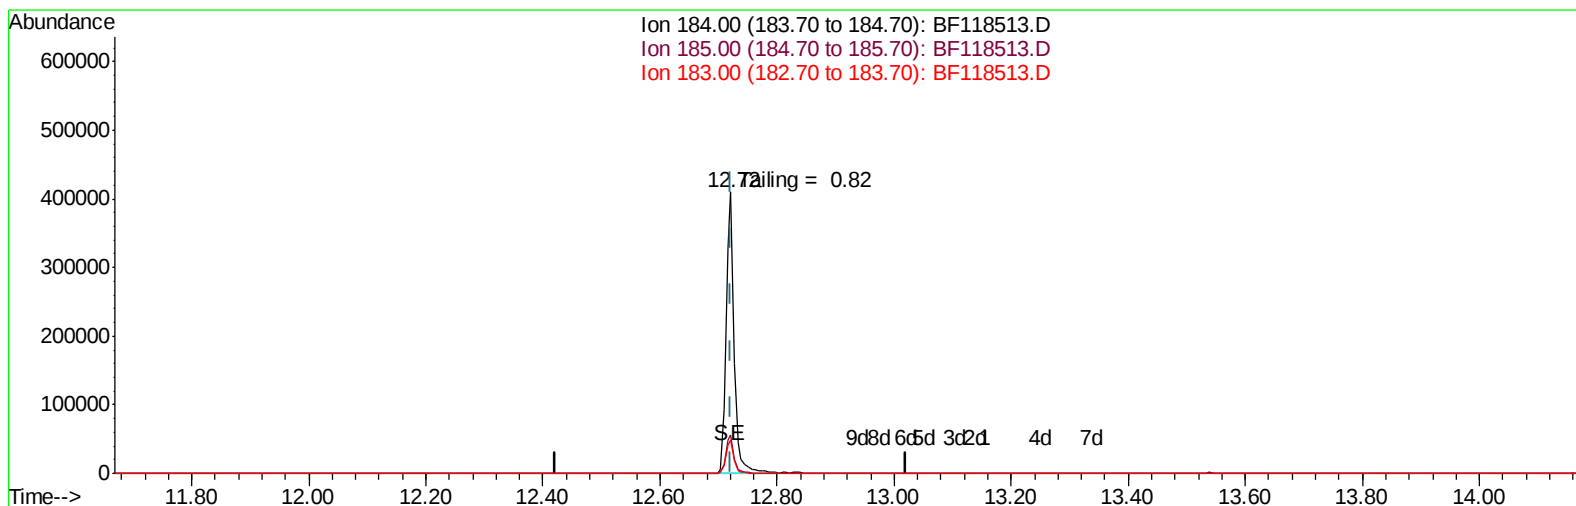

TIC: BF118513.D

(77) Benzidine

13.157min (+0.436) -1.00ng

response 106

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00