


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011020\
 Data File : BF118513.D
 Acq On : 10 Jan 2020 11:45
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 16:06:11 2020

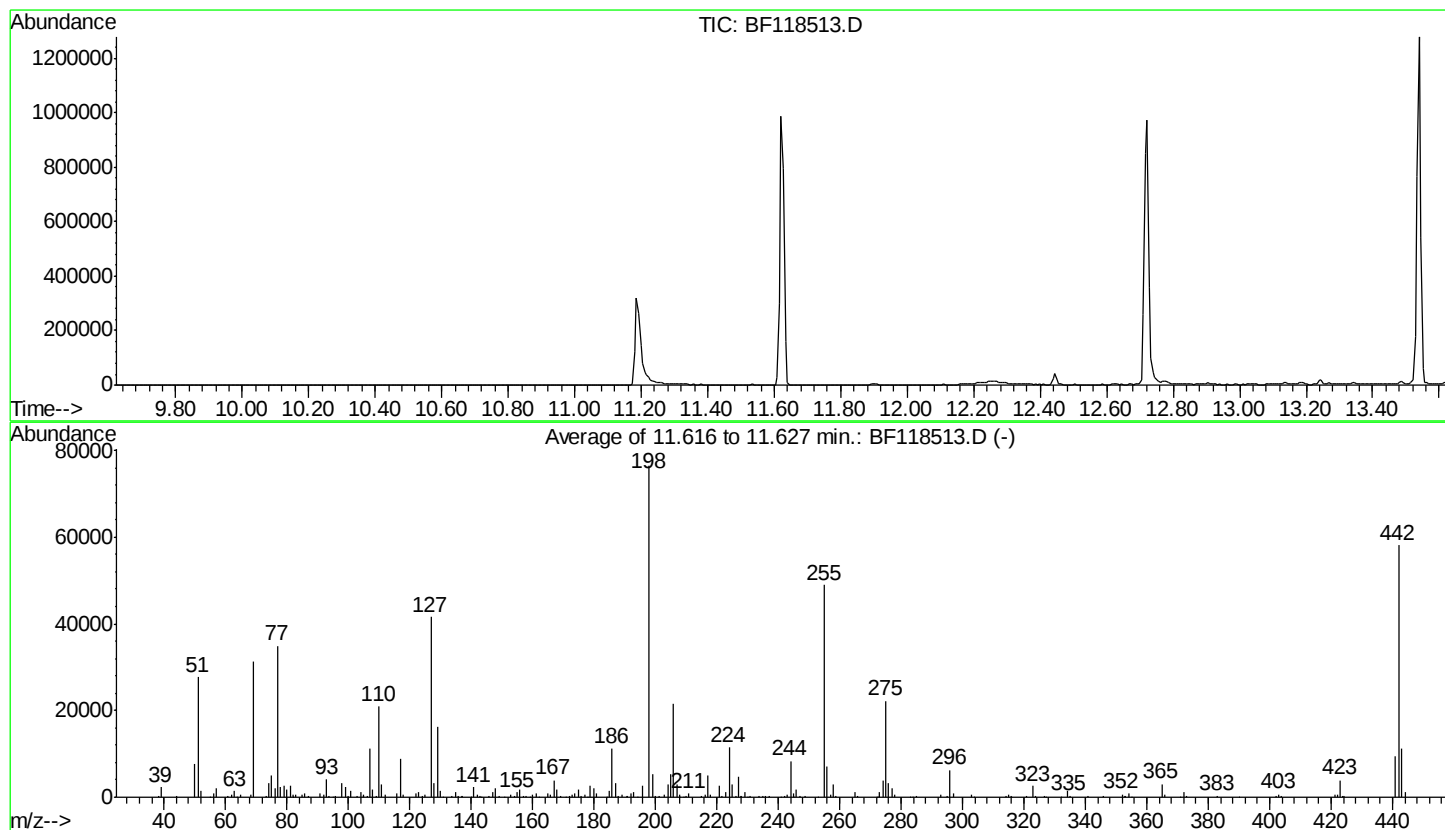

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	27706	PASS
68	69	0.00	2	1.6	511	PASS
69	198	0.00	100	40.7	31170	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	41560	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76498	PASS
199	198	5	9	6.9	5290	PASS
275	198	10	60	29.0	22149	PASS
365	198	1	100	4.0	3061	PASS
441	198	0.01	100	12.5	9581	PASS
442	198	50	100	76.0	58118	PASS
443	442	15	24	19.3	11204	PASS