
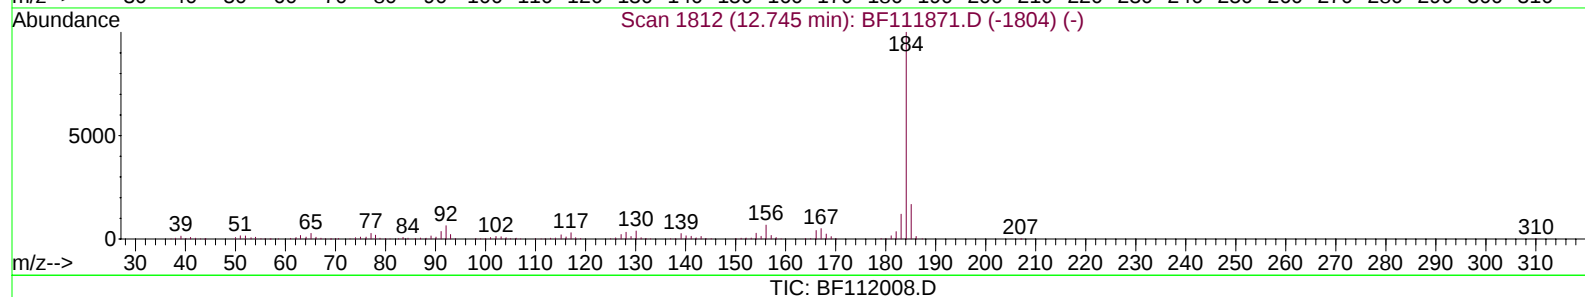
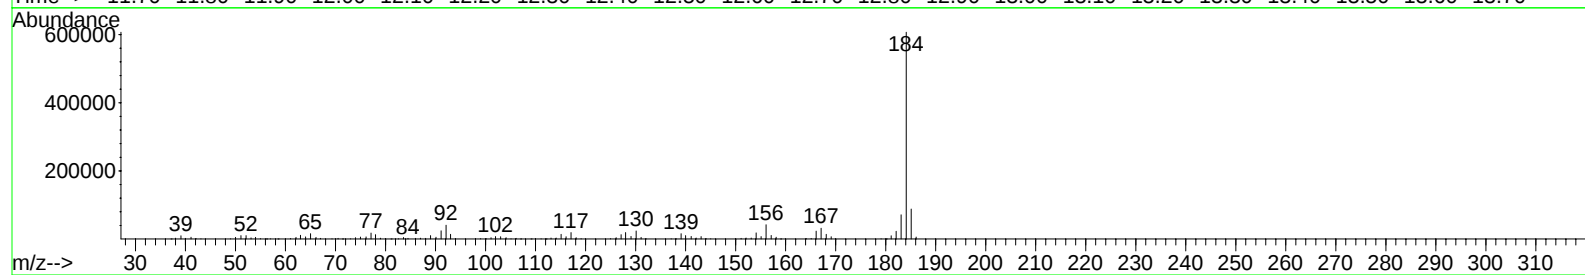


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011119\
Data File : BF112008.D
Acq On : 11 Jan 2019 12:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 12:58:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 11 21:37:26 2019
Response via : Initial Calibration

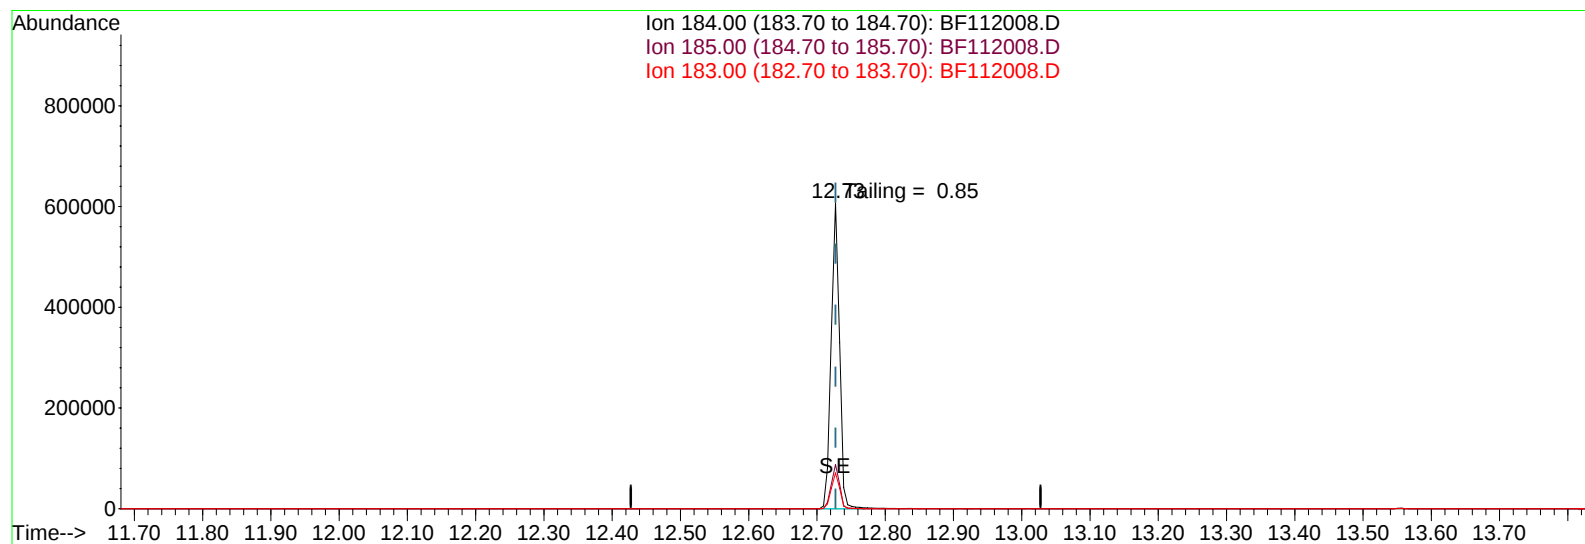

(77) Benzidine




12.727min (-0.000) 0.00ng

response 513081

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.52
183.00	12.00	11.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011119\
Data File : BF112008.D
Acq On : 11 Jan 2019 12:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 12:58:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 11 21:37:26 2019
Response via : Initial Calibration

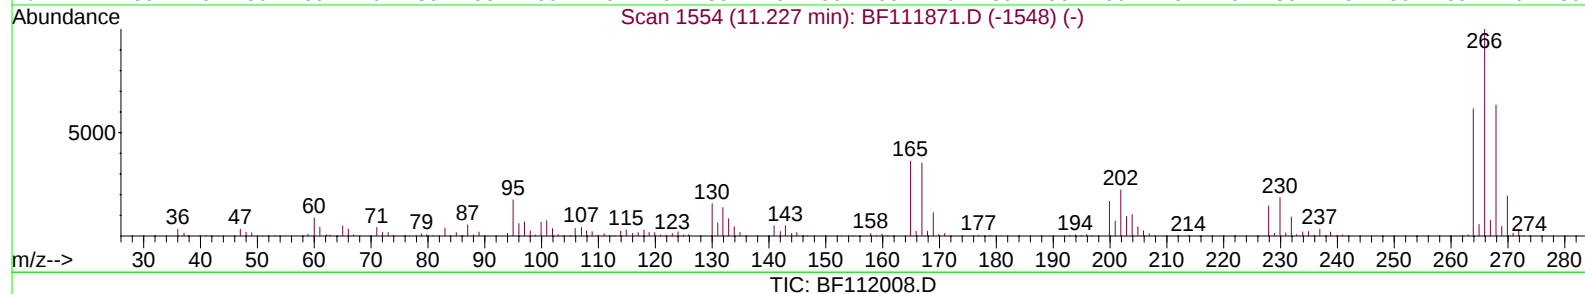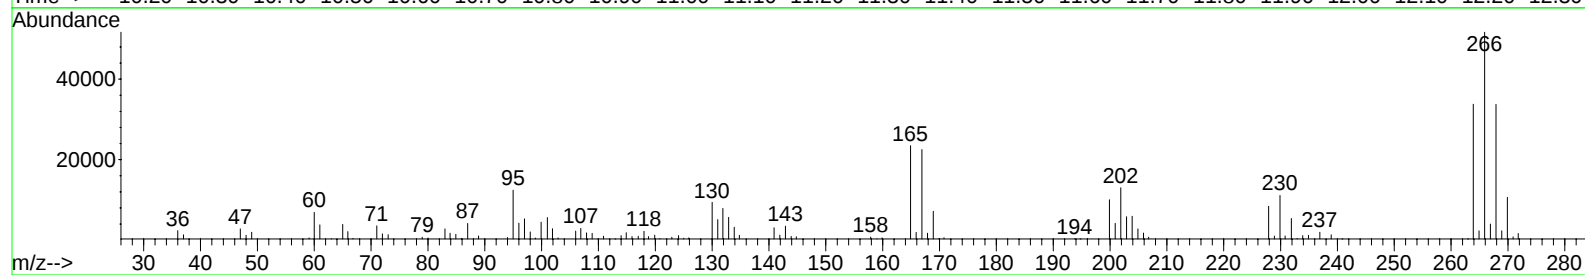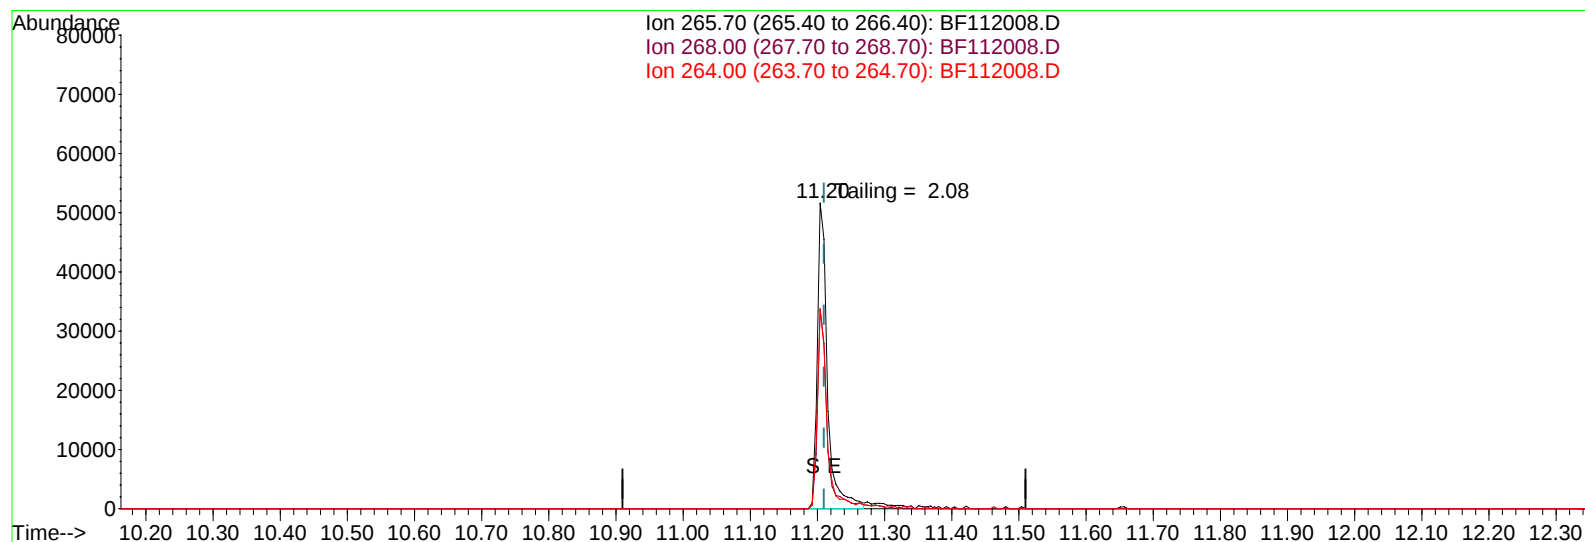

(70) Pentachlorophenol (C)

11.204min (-0.006) 21095.34ng

response 57381

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	65.28
264.00	61.60	65.39
0.00	0.00	0.00