
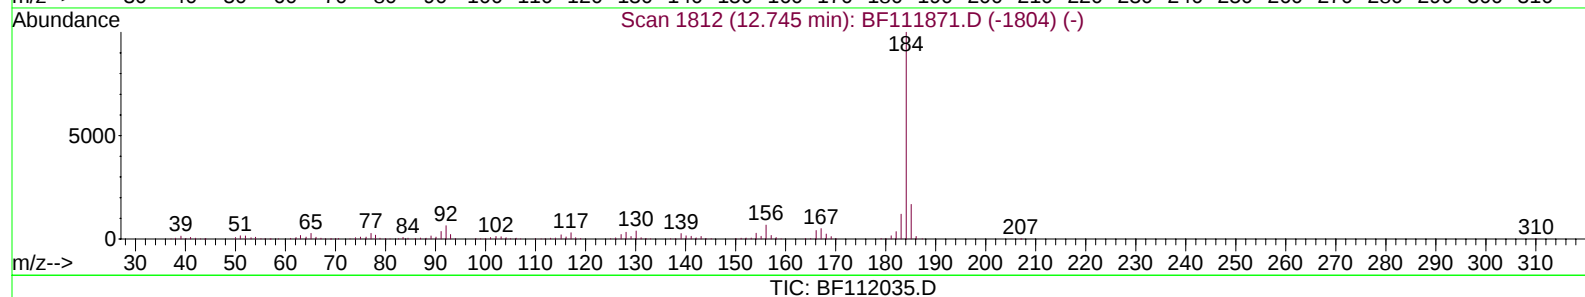
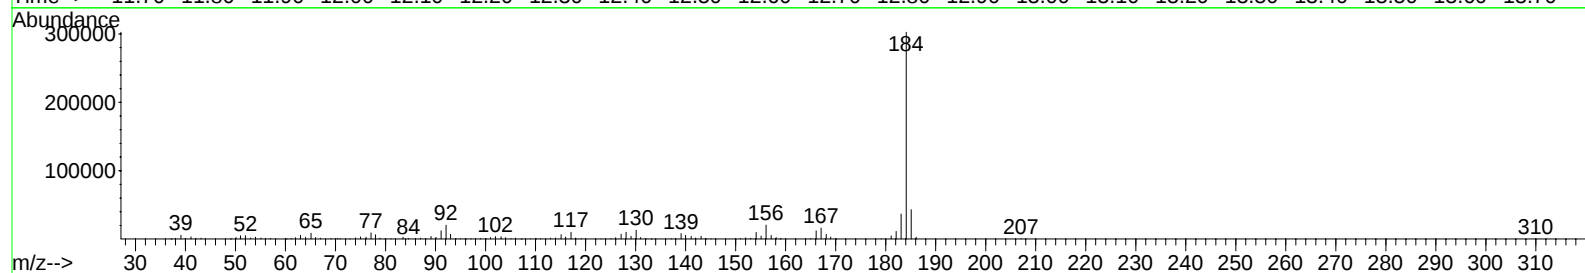


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011119\
Data File : BF112035.D
Acq On : 12 Jan 2019 00:45
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 12:54:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 11 21:37:26 2019
Response via : Initial Calibration

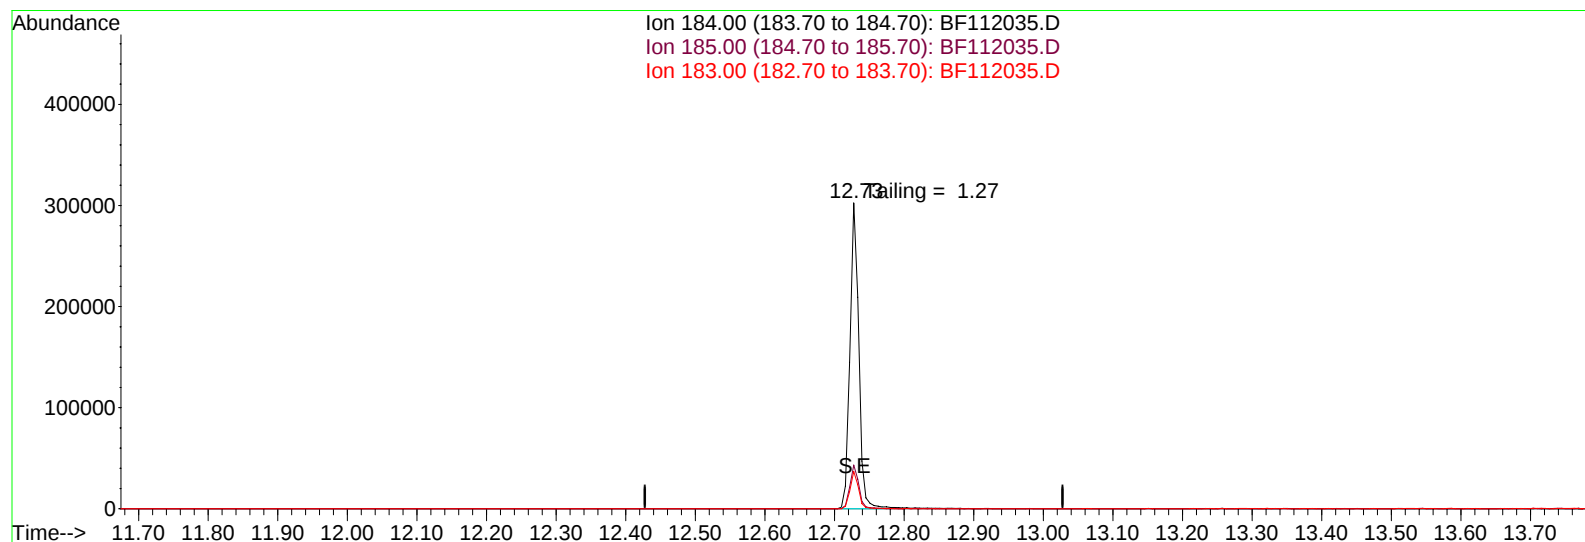

TIC: BF112035.D

(77) Benzidine




12.727min (-12.727) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.70	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011119\
Data File : BF112035.D
Acq On : 12 Jan 2019 00:45
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 12:54:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 11 21:37:26 2019
Response via : Initial Calibration

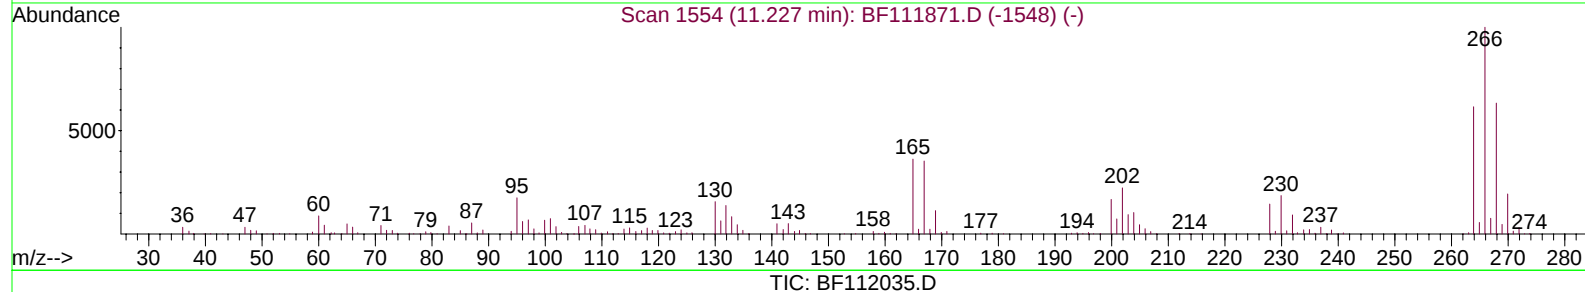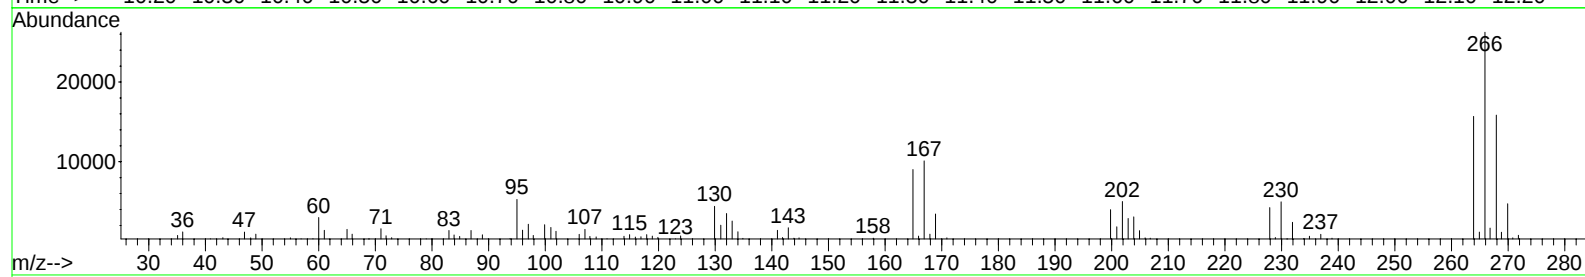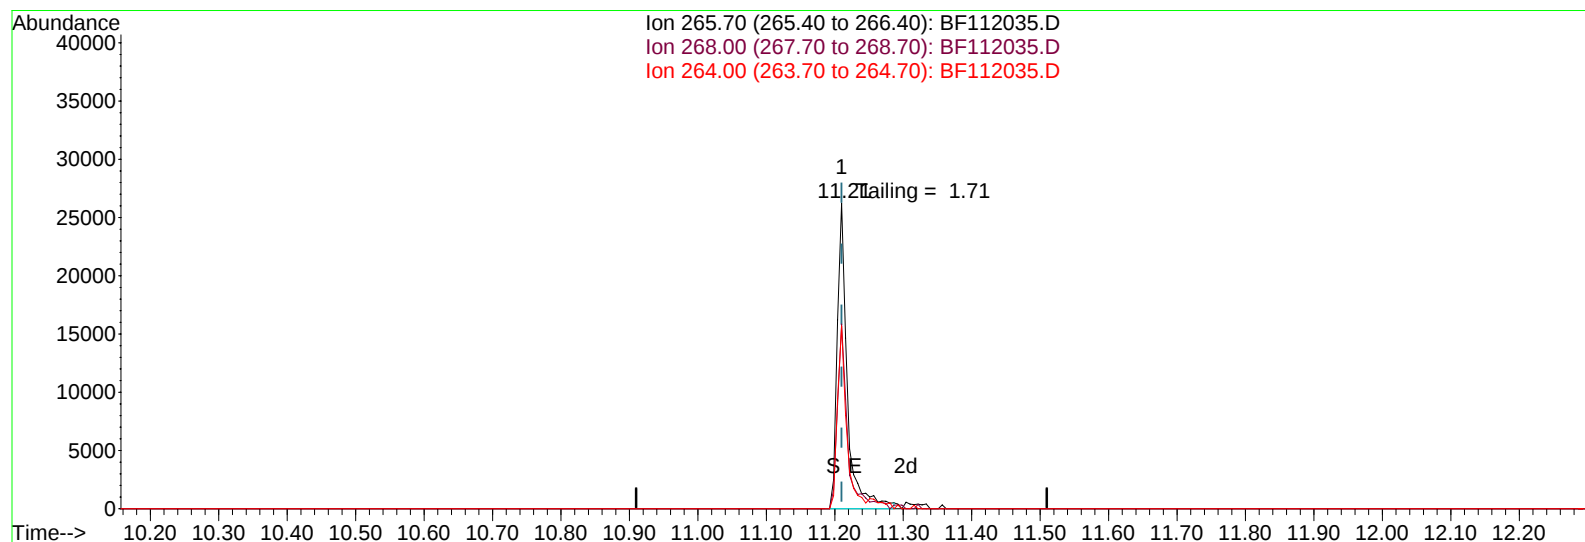

(70) Pentachlorophenol (C)

11.210min (-0.000) 13342.16ng

response 27464

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	60.37
264.00	61.60	59.75
0.00	0.00	0.00