


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011119\
 Data File : BF112008.D
 Acq On : 11 Jan 2019 12:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 11 21:37:26 2019

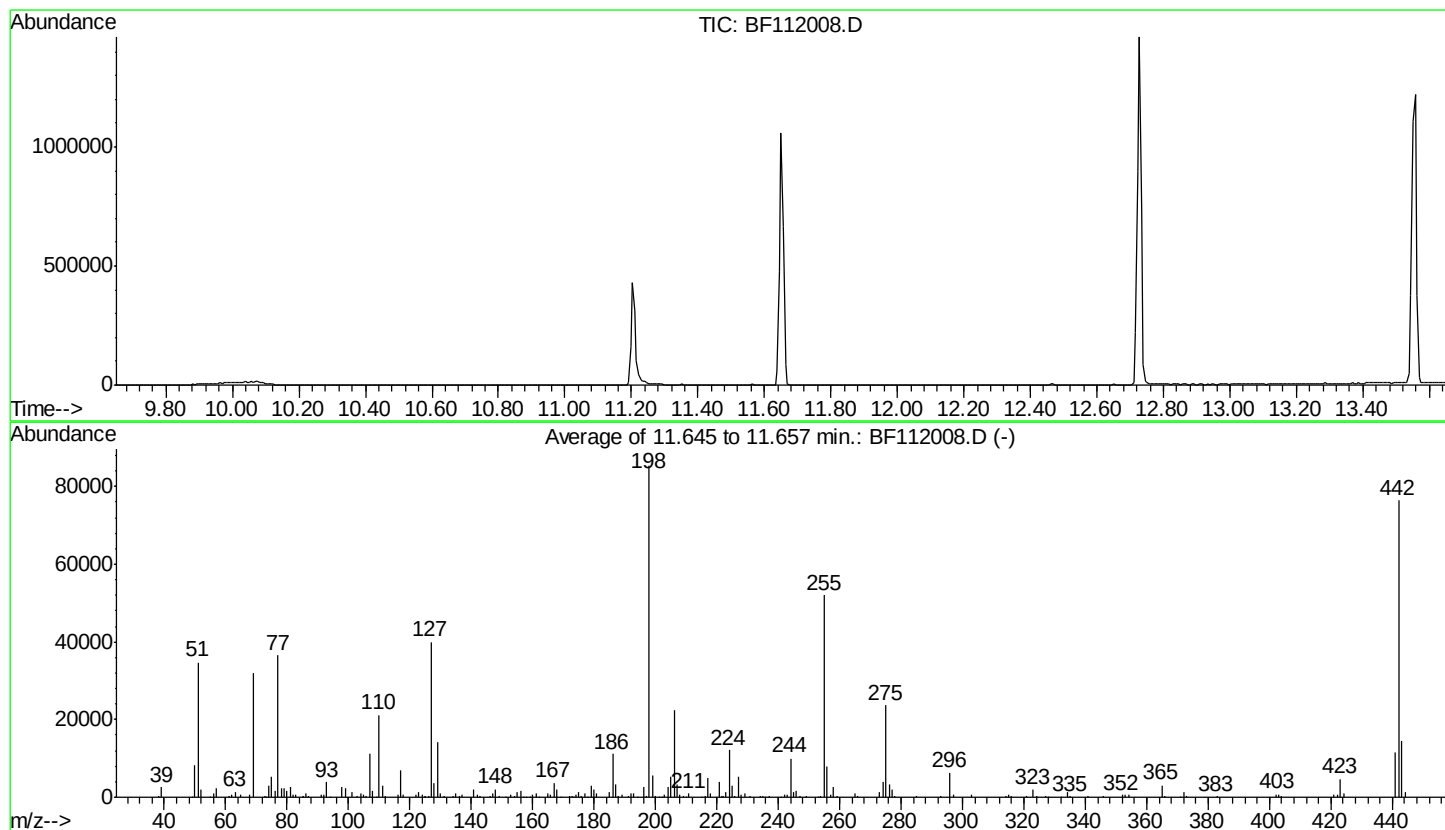

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	34648	PASS
68	69	0.00	2	1.9	613	PASS
69	198	0.00	100	37.3	31880	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	39997	PASS
197	198	0.00	2	0.5	404	PASS
198	198	100	100	100.0	85381	PASS
199	198	5	9	6.7	5760	PASS
275	198	10	60	27.7	23670	PASS
365	198	1	100	3.6	3112	PASS
441	198	0.01	100	13.4	11433	PASS
442	198	50	100	89.5	76437	PASS
443	442	15	24	19.0	14553	PASS