
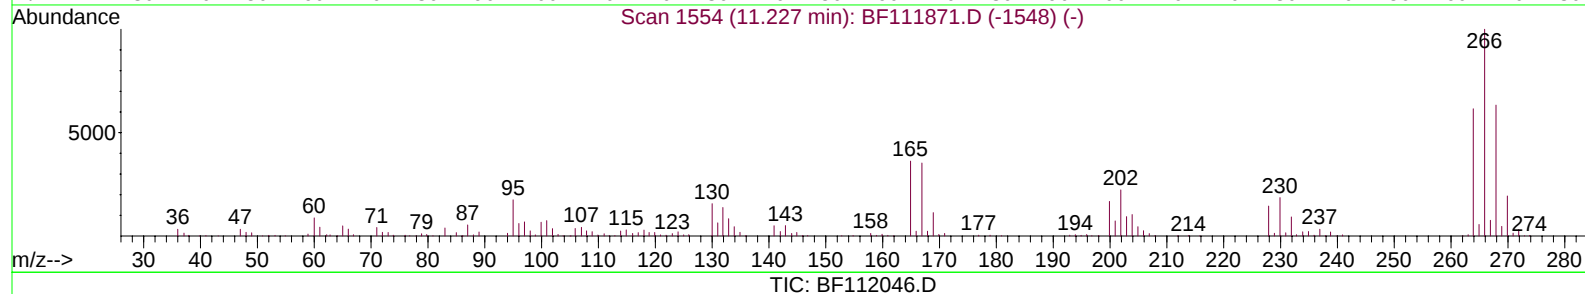
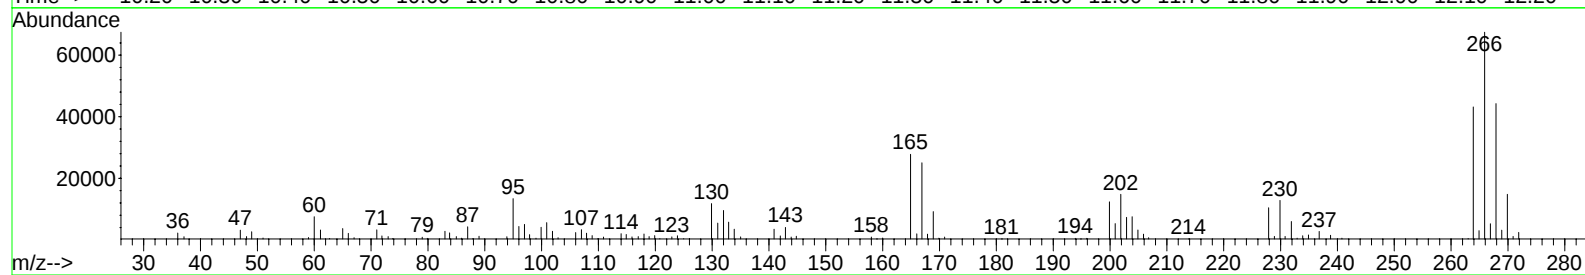


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011419\
Data File : BF112046.D
Acq On : 14 Jan 2019 13:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 18:12:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 11 21:37:26 2019
Response via : Initial Calibration

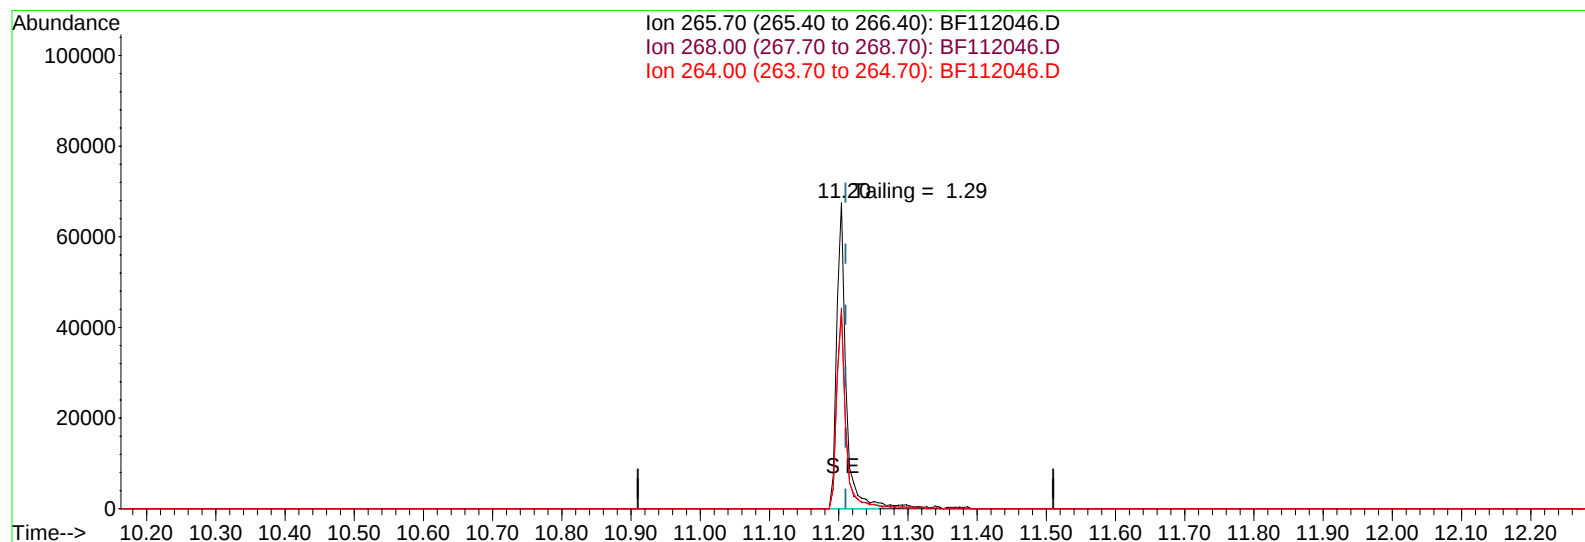

(70) Pentachlorophenol (C)




11.204min (-0.006) 43053.42ng

response 63302

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	65.62
264.00	61.60	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011419\
Data File : BF112046.D
Acq On : 14 Jan 2019 13:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 14 18:12:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 11 21:37:26 2019
Response via : Initial Calibration

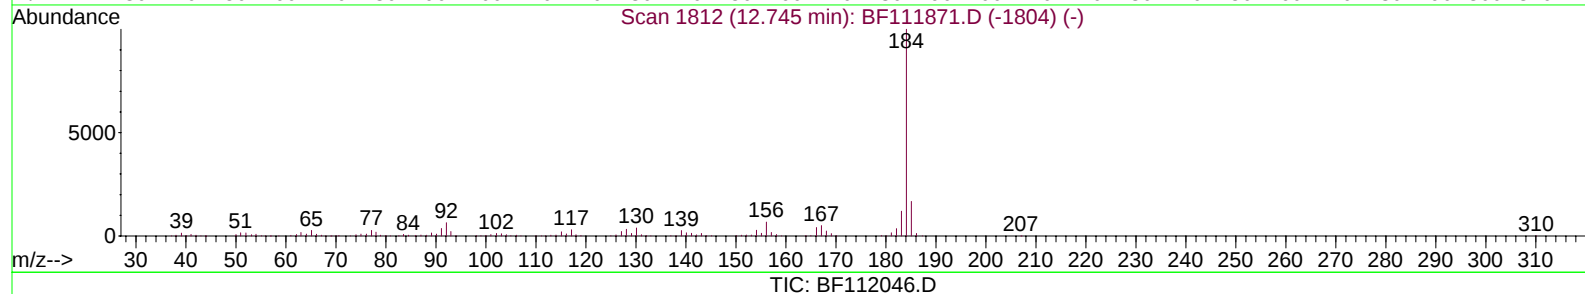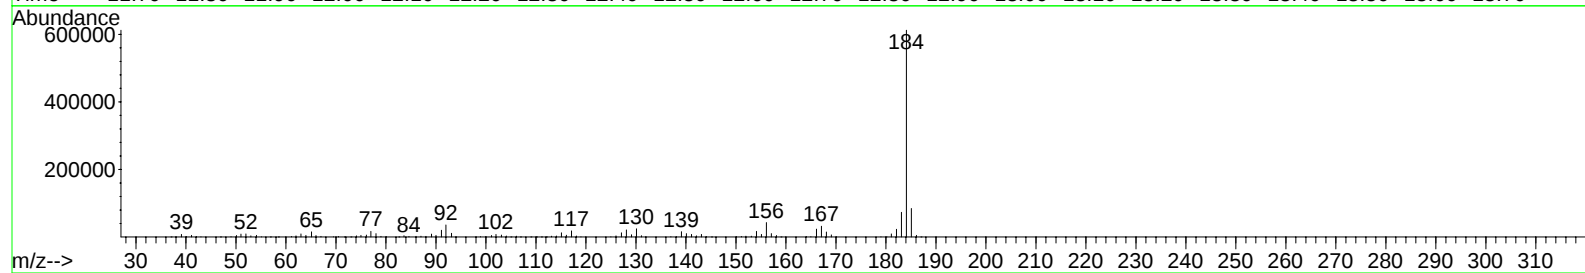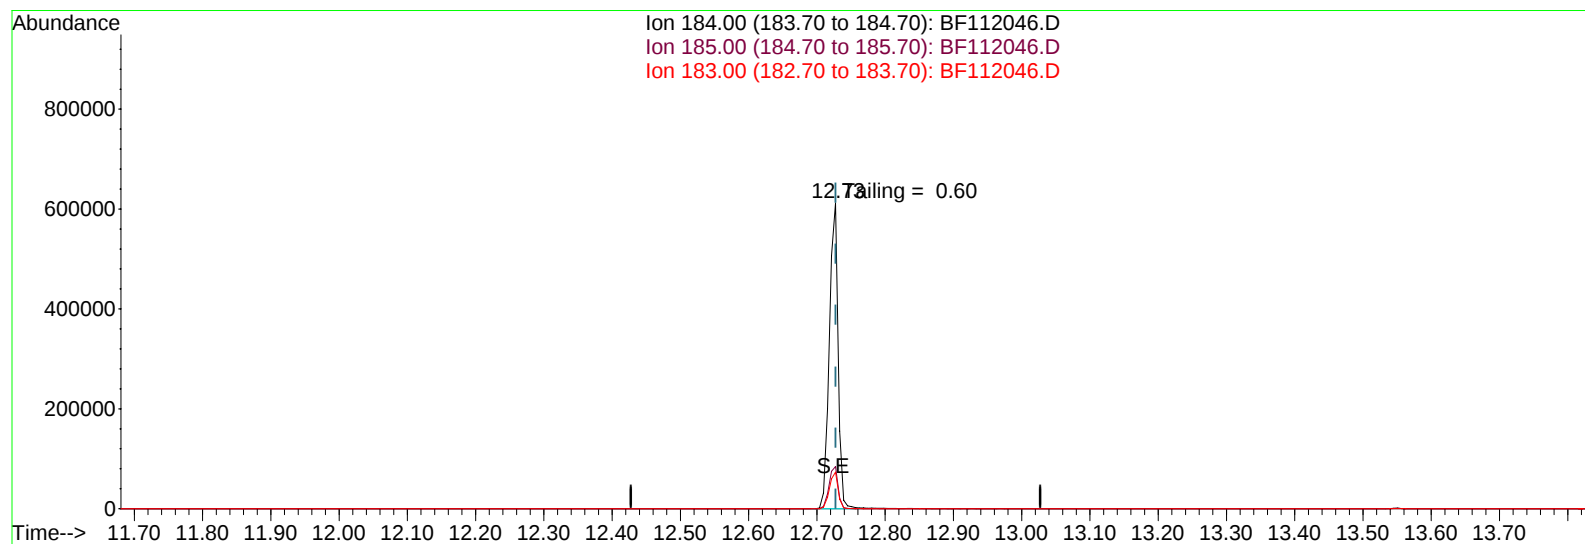

(77) Benzidine

12.727min (-0.000) 0.00ng

response 545866

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	13.83
183.00	12.00	11.98
0.00	0.00	0.00