

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011419\
 Data File : BF112061.D
 Acq On : 14 Jan 2019 20:02
 Operator : JU/SJ
 Sample : K1015-07 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-011119-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	503	507	511	rVB	22399	23890	2.55%	0.263%
2	5.498	576	580	591	rBV	459357	409944	43.79%	4.511%
3	6.510	748	752	767	rBV	458679	449812	48.05%	4.949%
4	6.639	771	774	781	rBV	547239	453545	48.45%	4.990%
5	6.869	809	813	816	rBV	816738	678124	72.44%	7.461%
6	7.022	836	839	843	rBV	449286	358842	38.33%	3.948%
7	7.422	904	907	913	rBV	336662	270438	28.89%	2.976%
8	8.151	1027	1031	1034	rBV	1093855	855717	91.41%	9.416%
9	8.739	1128	1131	1136	rBV2	16883	13547	1.45%	0.149%
10	9.222	1210	1213	1216	rBV	805966	607610	64.91%	6.686%
11	9.304	1224	1227	1230	rBV2	28372	27870	2.98%	0.307%
12	9.492	1255	1259	1263	rBV3	9899	13595	1.45%	0.150%
13	9.563	1267	1271	1273	rVV	15681	14123	1.51%	0.155%
14	9.610	1277	1279	1284	rVB	121668	114029	12.18%	1.255%
15	9.833	1315	1317	1320	rVB	24657	19022	2.03%	0.209%
16	9.904	1326	1329	1333	rVB2	1097710	935758	99.96%	10.296%
17	10.110	1359	1364	1368	rBV3	11826	12965	1.38%	0.143%
18	10.151	1368	1371	1376	rVB3	10357	13095	1.40%	0.144%
19	10.333	1399	1402	1405	rVB	32298	24479	2.61%	0.269%
20	10.557	1435	1440	1445	rVB4	13370	20343	2.17%	0.224%
21	10.692	1460	1463	1468	rBV	333067	271703	29.02%	2.990%
22	10.804	1479	1482	1489	rVB2	41665	65266	6.97%	0.718%
23	11.257	1554	1559	1562	rBV2	33300	37778	4.04%	0.416%
24	11.286	1562	1564	1567	rVB	22119	16514	1.76%	0.182%
25	11.392	1578	1582	1585	rBV	1070192	861398	92.02%	9.478%
26	11.416	1585	1586	1589	rVB	29446	14985	1.60%	0.165%
27	11.680	1626	1631	1634	rBV	35216	32851	3.51%	0.361%
28	12.004	1683	1686	1688	rBV4	10749	11685	1.25%	0.129%
29	12.086	1695	1700	1704	rBV2	39271	71312	7.62%	0.785%
30	12.210	1719	1721	1725	rBV4	11325	18308	1.96%	0.201%
31	12.321	1737	1740	1746	rVB7	30110	42598	4.55%	0.469%
32	12.445	1758	1761	1763	rBV2	14542	17672	1.89%	0.194%
33	12.480	1763	1767	1772	rVB6	30765	41700	4.45%	0.459%
34	12.604	1786	1788	1791	rBV	35384	30558	3.26%	0.336%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011419\
Data File : BF112061.D
Acq On : 14 Jan 2019 20:02
Operator : JU/SJ
Sample : K1015-07 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-011119-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.704	1802	1805	1807	rBV4	17851	24103	2.57%	0.265%
36	12.839	1825	1828	1833	rBV3	43084	68624	7.33%	0.755%
37	12.974	1847	1851	1854	rBV	469321	400173	42.75%	4.403%
38	14.033	2027	2031	2034	rBV	913240	808272	86.34%	8.893%
39	15.515	2279	2283	2293	rVB2	568206	936122	100.00%	10.300%


Sum of corrected areas: 9088370

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011419\
Data File : BF112061.D
Acq On : 14 Jan 2019 20:02
Operator : JU/SJ
Sample : K1015-07 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-011119-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

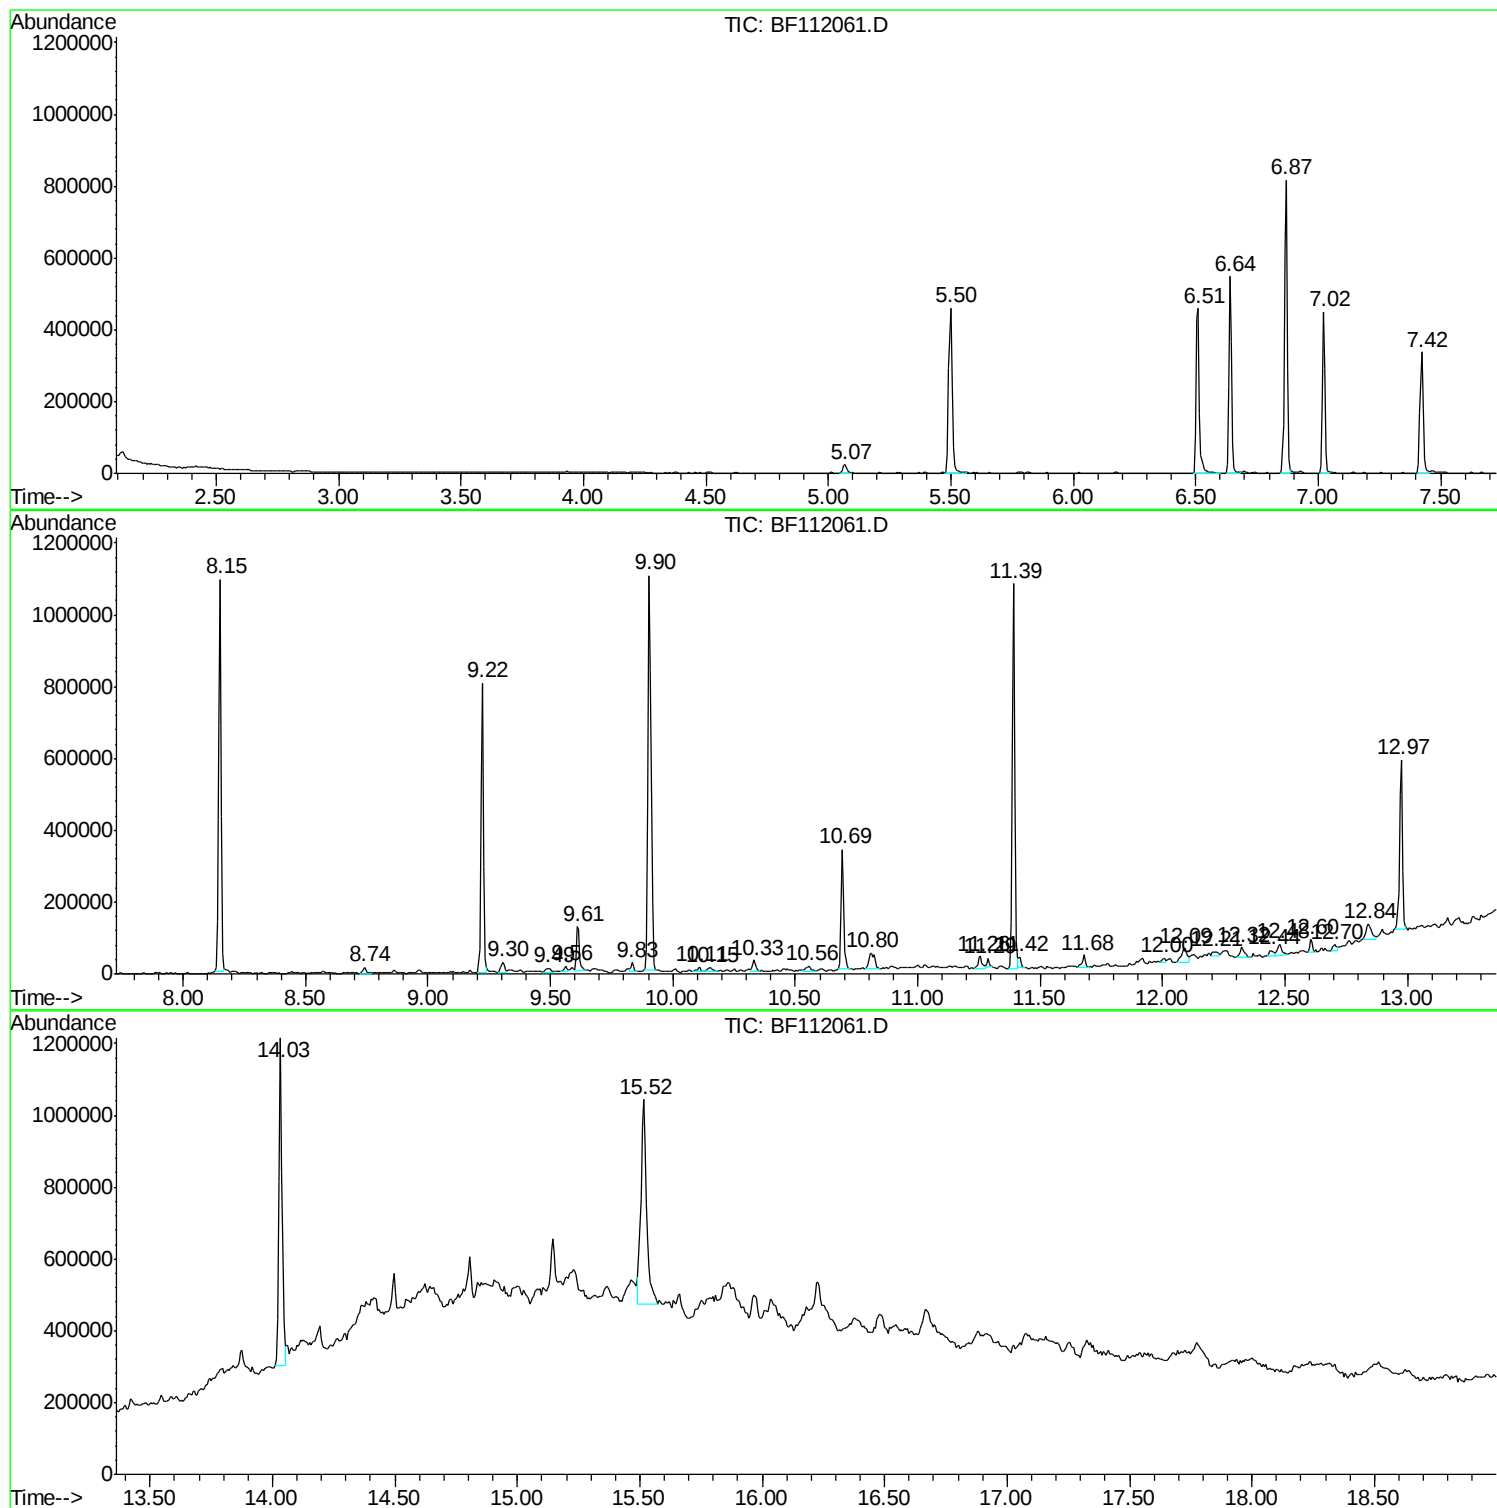

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011419\
Data File : BF112061.D
Acq On : 14 Jan 2019 20:02
Operator : JU/SJ
Sample : K1015-07 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-011119-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.64 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.64	13.38 ng	453545	1,4-Dichlorobenzene-d4	6.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

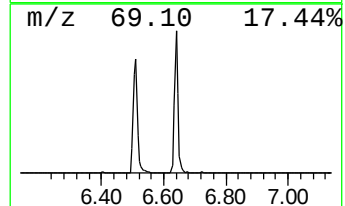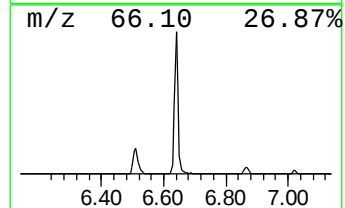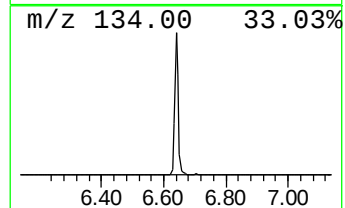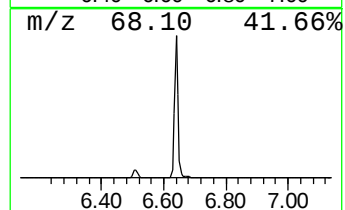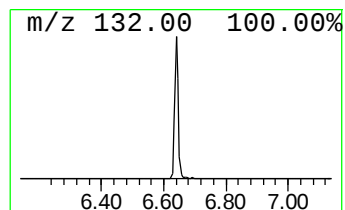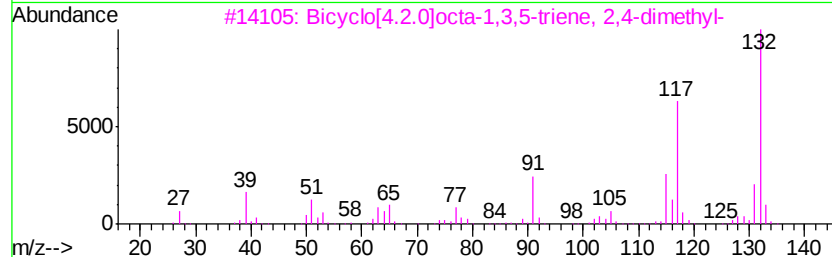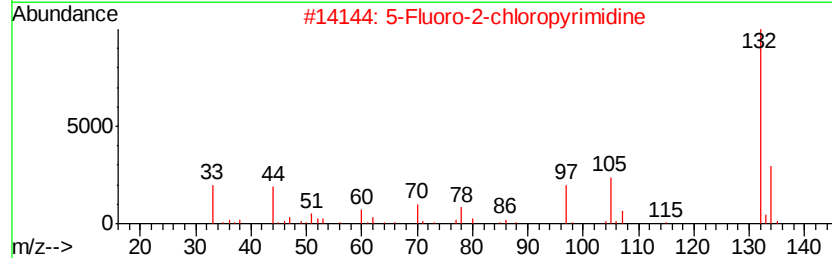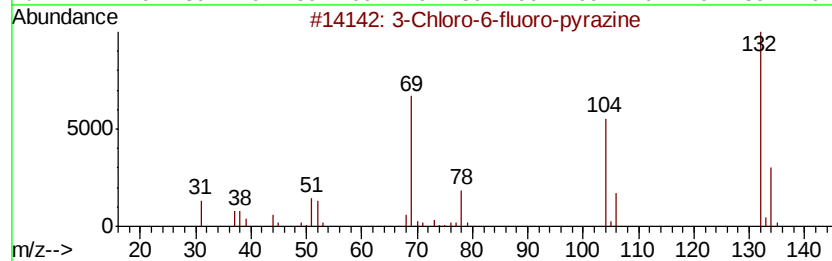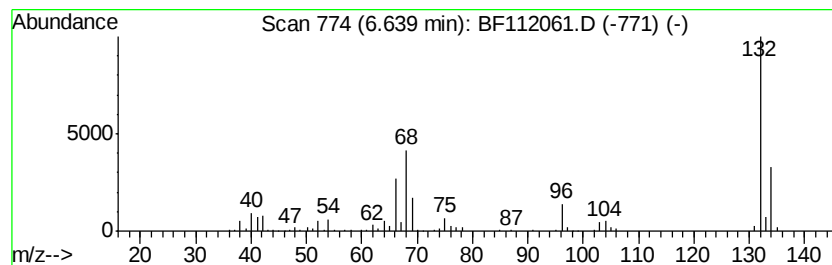

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011419\
Data File : BF112061.D
Acq On : 14 Jan 2019 20:02
Operator : JU/SJ
Sample : K1015-07 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-011119-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.64	6.64	13.4	ng	453545	1	6.87	678124	20.0