
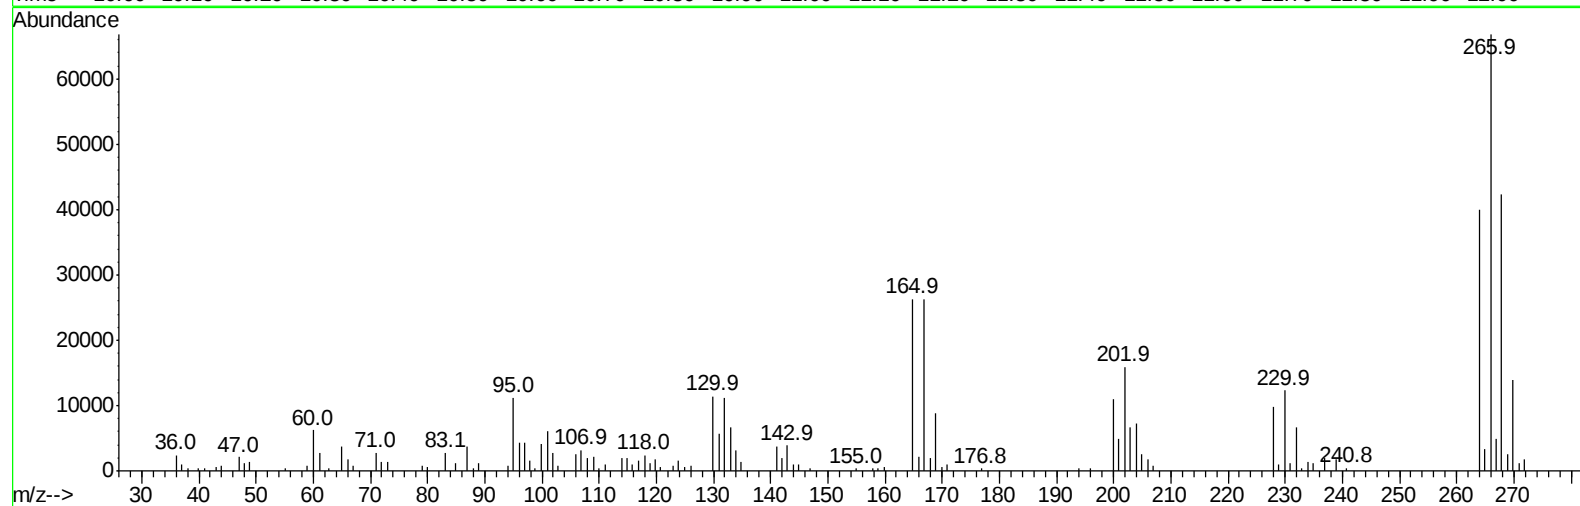


Data Path : U:\HPCHEM1\BNA F\DATA\BF011518\
Data File : BF102089.D
Acq On : 16 Jan 2018 3:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:35:55 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

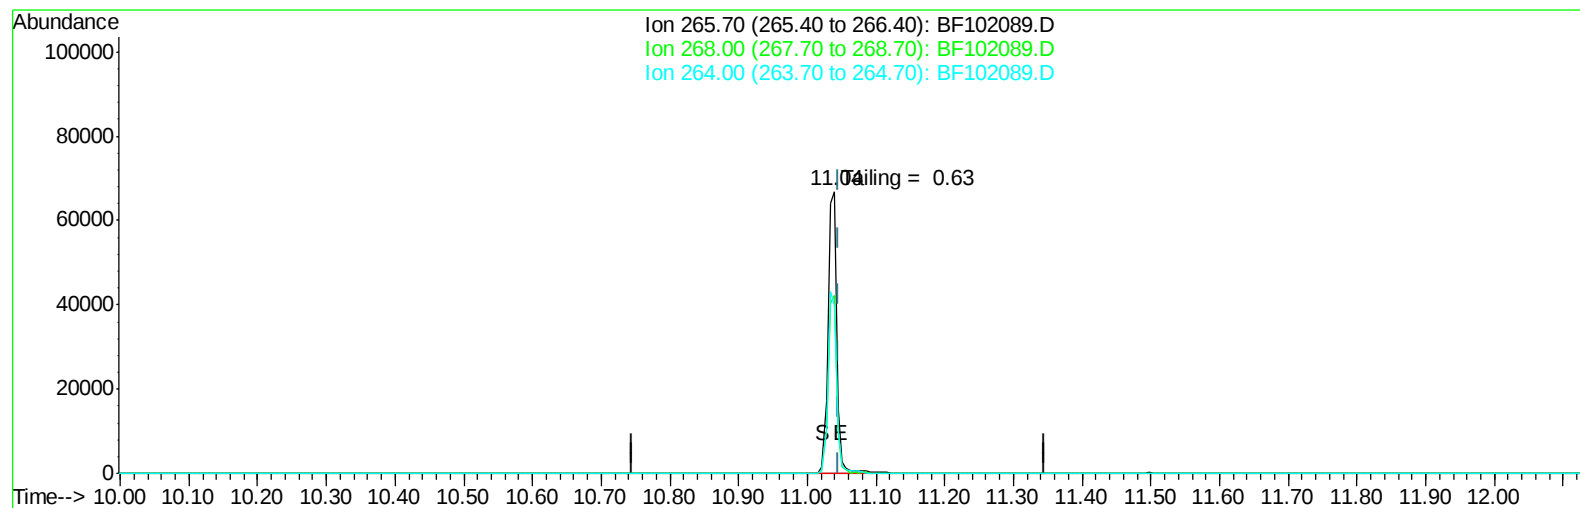

TIC: BF102089.D

(69) Pentachlorophenol (C)



11.039min (-0.006) 45178.75ng

response 61299

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.34
264.00	61.90	59.77
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011518\
Data File : BF102089.D
Acq On : 16 Jan 2018 3:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:35:55 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

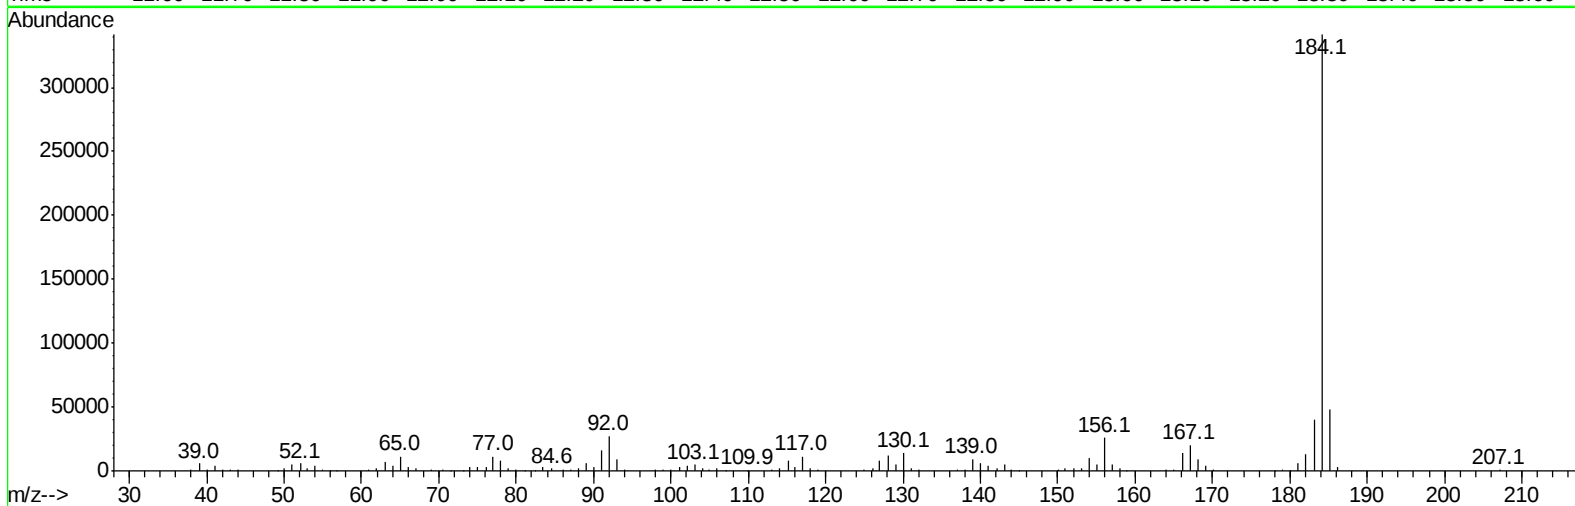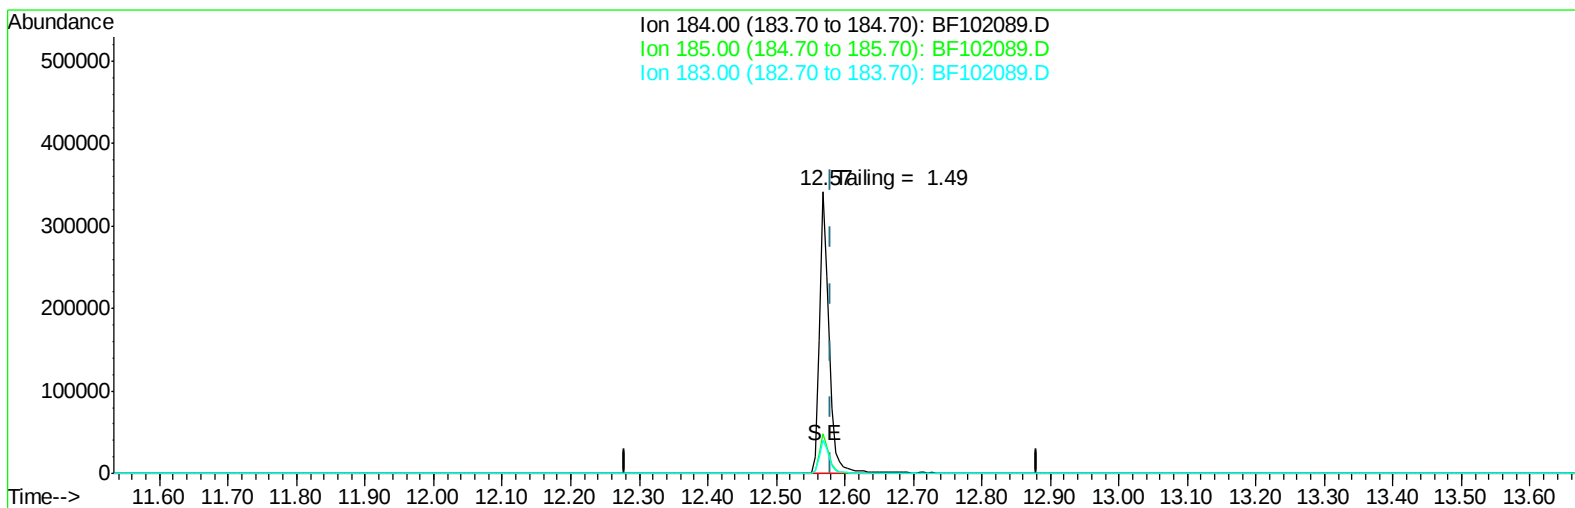

TIC: BF102089.D

(76) Benzidine

12.568min (-0.012) 0.00ng

response 325762

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.99
183.00	11.60	11.85
0.00	0.00	0.00