


Data Path : U:\HPCHEM1\BNA F\Data\BF011518\
 Data File : BF102062.D
 Acq On : 15 Jan 2018 14:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 15 10:05:15 2018

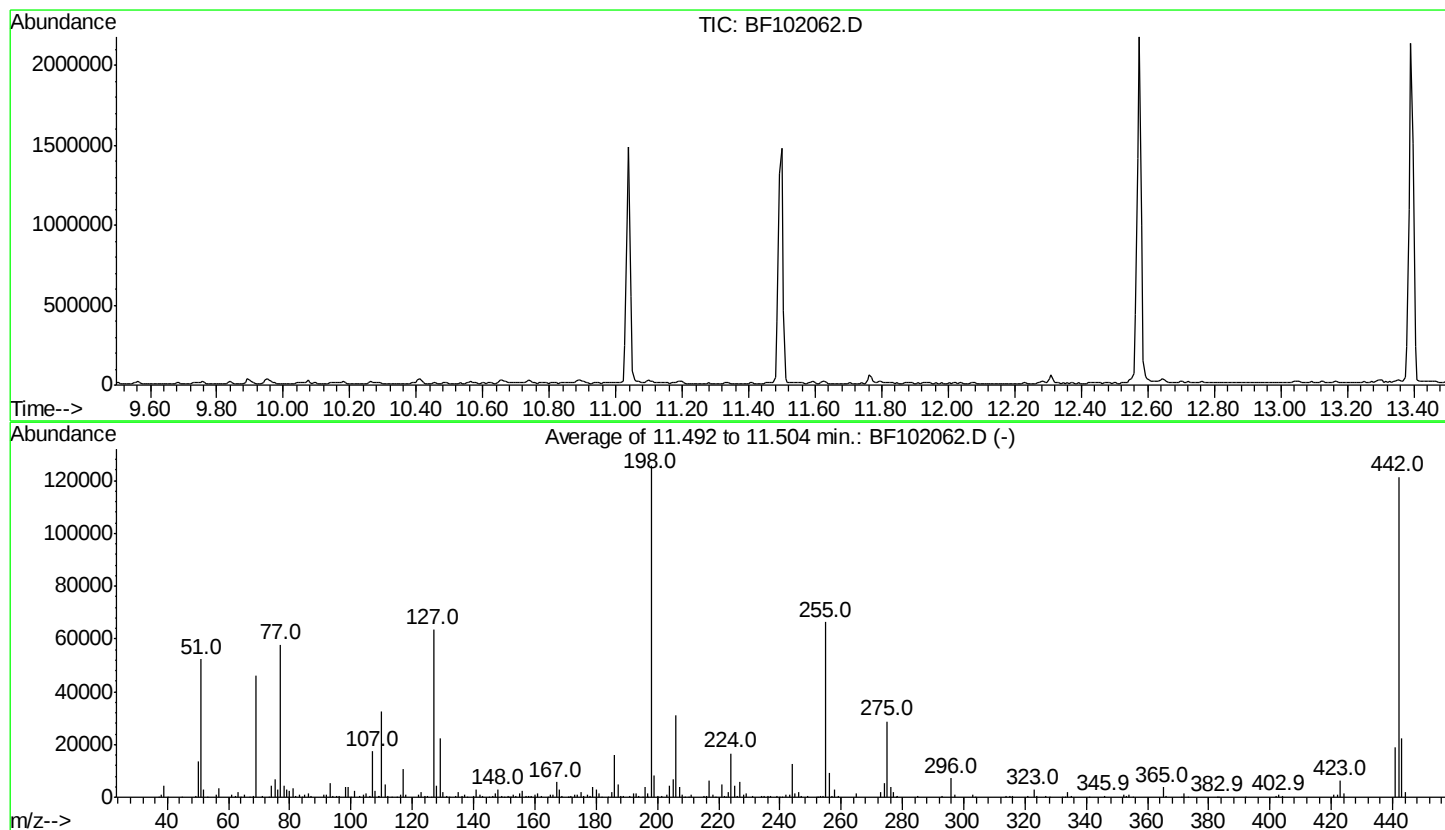

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	52193	PASS
68	69	0.00	2	1.2	545	PASS
69	198	0.00	100	36.6	46018	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	63392	PASS
197	198	0.00	2	1.0	1307	PASS
198	198	100	100	100.0	125618	PASS
199	198	5	9	6.6	8352	PASS
275	198	10	60	22.8	28635	PASS
365	198	1	100	3.1	3874	PASS
441	442	0.01	24	15.7	19034	PASS
442	198	50	100	96.6	121344	PASS
443	442	15	24	18.3	22181	PASS