


Data Path : U:\HPCHEM1\BNA_F\Data\BF011518\
 Data File : BF102089.D
 Acq On : 16 Jan 2018 3:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 11 12:53:54 2018

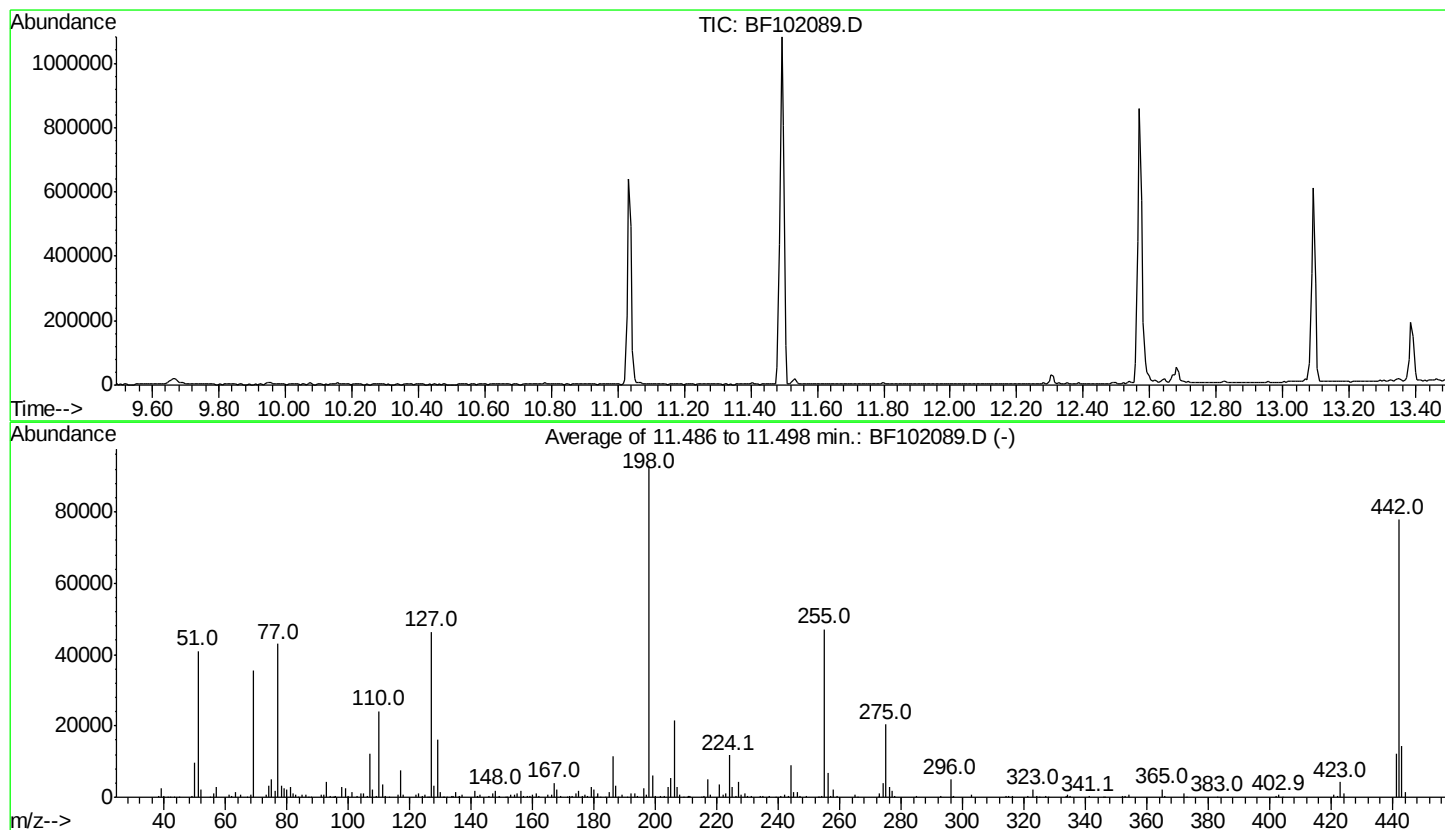

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	41048	PASS
68	69	0.00	2	1.7	613	PASS
69	198	0.00	100	38.1	35432	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	46453	PASS
197	198	0.00	2	0.7	628	PASS
198	198	100	100	100.0	92949	PASS
199	198	5	9	6.8	6288	PASS
275	198	10	60	21.9	20346	PASS
365	198	1	100	2.4	2261	PASS
441	443	0.01	100	85.4	12222	PASS
442	198	50	100	83.6	77717	PASS
443	442	15	24	18.4	14308	PASS