


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011619\
 Data File : BF112065.D
 Acq On : 16 Jan 2019 14:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 16 18:22:05 2019

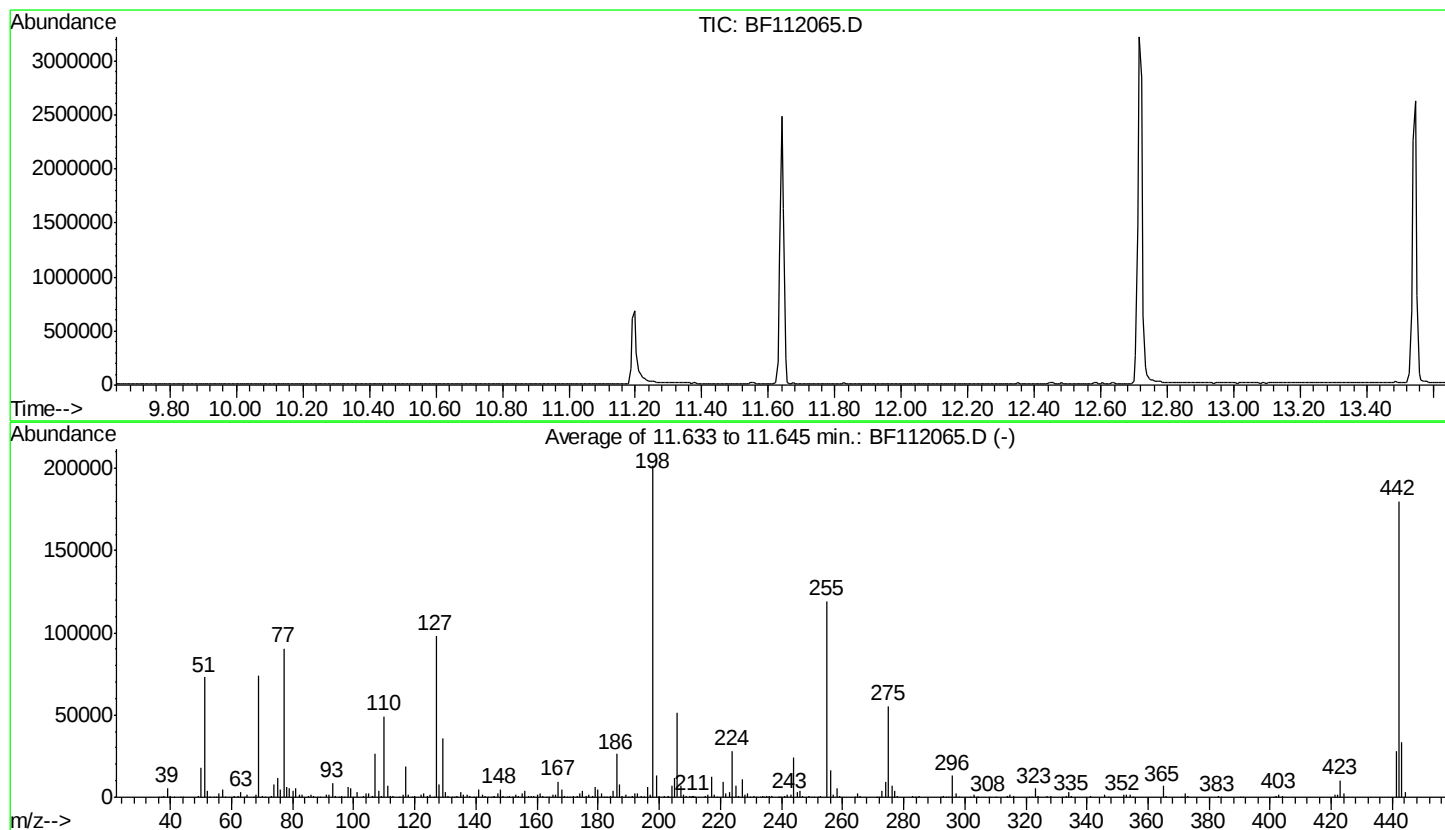

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	72853	PASS
68	69	0.00	2	2.0	1455	PASS
69	198	0.00	100	36.6	73872	PASS
70	69	0.00	2	0.9	680	PASS
127	198	10	80	48.6	98090	PASS
197	198	0.00	2	0.8	1682	PASS
198	198	100	100	100.0	201664	PASS
199	198	5	9	6.7	13527	PASS
275	198	10	60	27.6	55626	PASS
365	198	1	100	3.3	6750	PASS
441	198	0.01	100	13.8	27767	PASS
442	198	50	100	89.3	180112	PASS
443	442	15	24	18.7	33607	PASS