
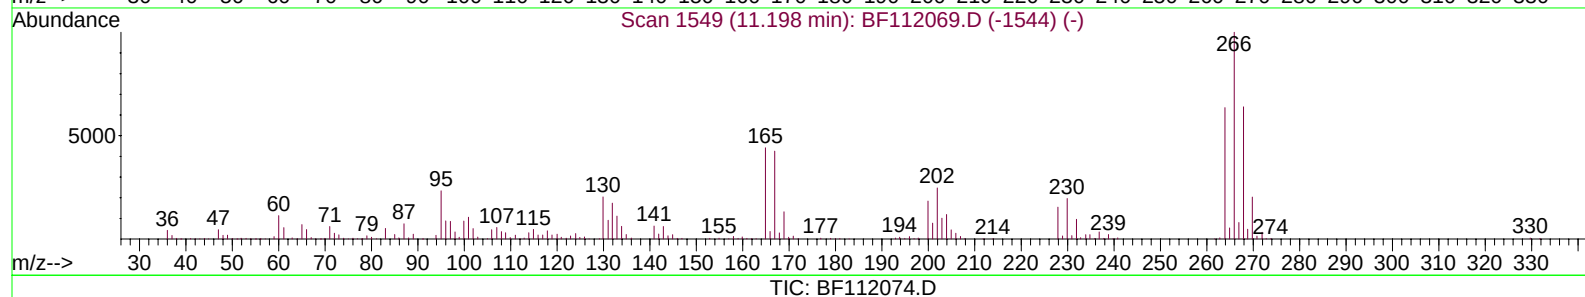
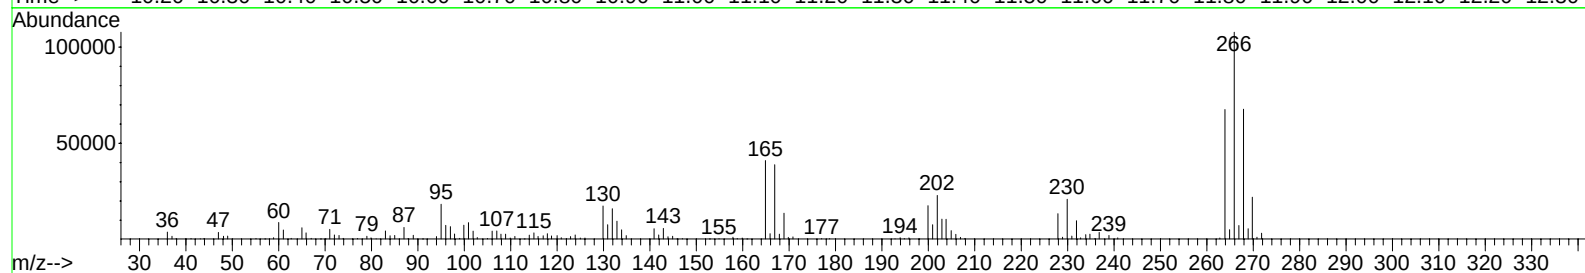


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011719\
Data File : BF112074.D
Acq On : 17 Jan 2019 8:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 17:57:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 16 18:22:05 2019
Response via : Initial Calibration

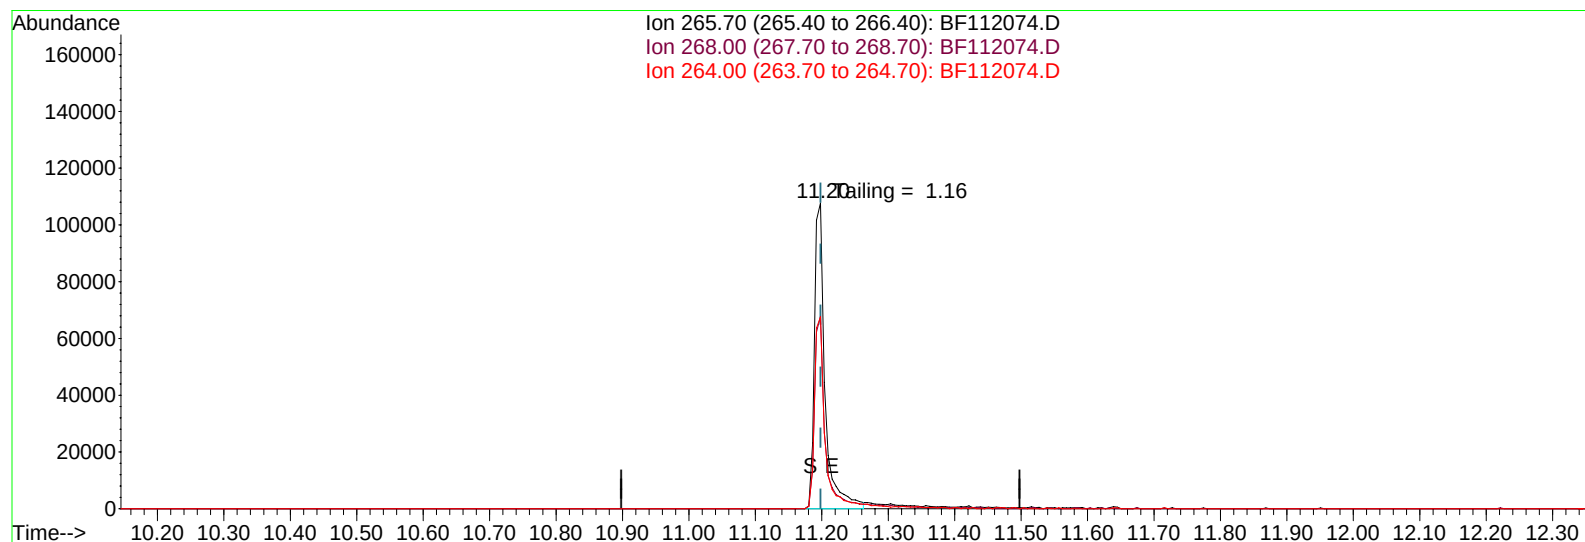

(70) Pentachlorophenol (C)




11.198min (-0.000) 19257.69ng

response 127768

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.90
264.00	63.60	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011719\
 Data File : BF112074.D
 Acq On : 17 Jan 2019 8:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 17:57:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 16 18:22:05 2019
 Response via : Initial Calibration

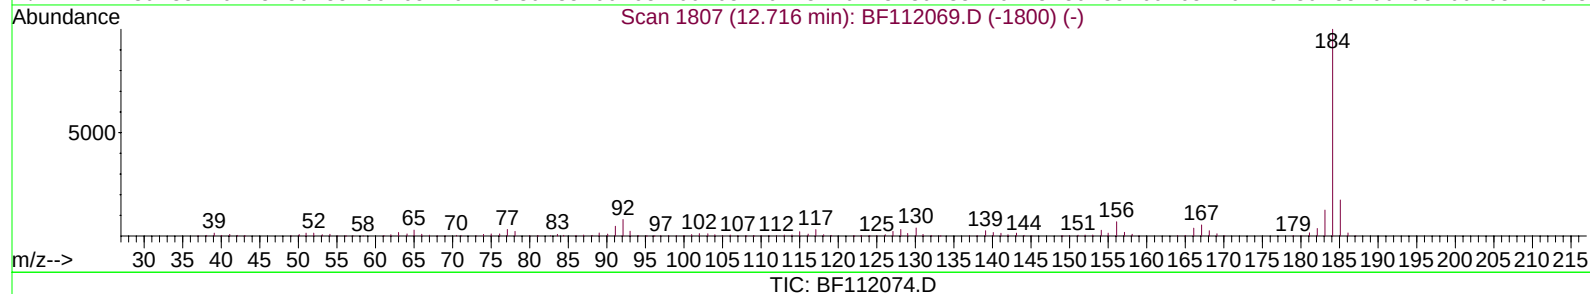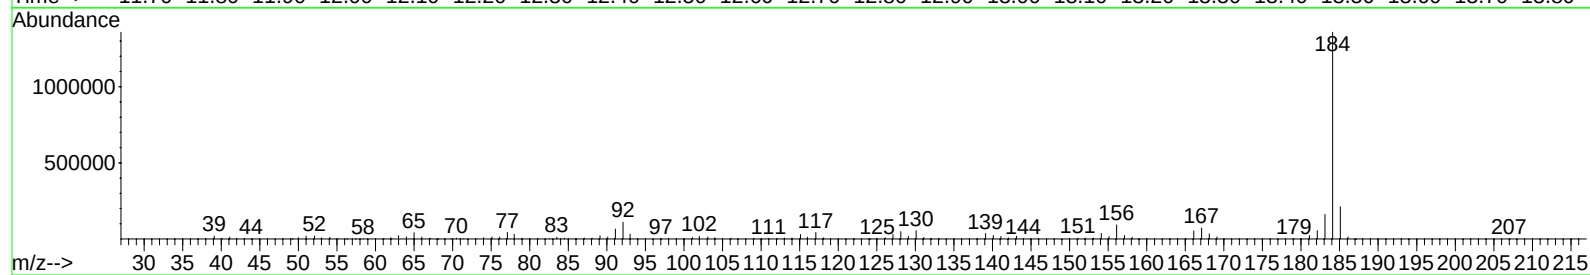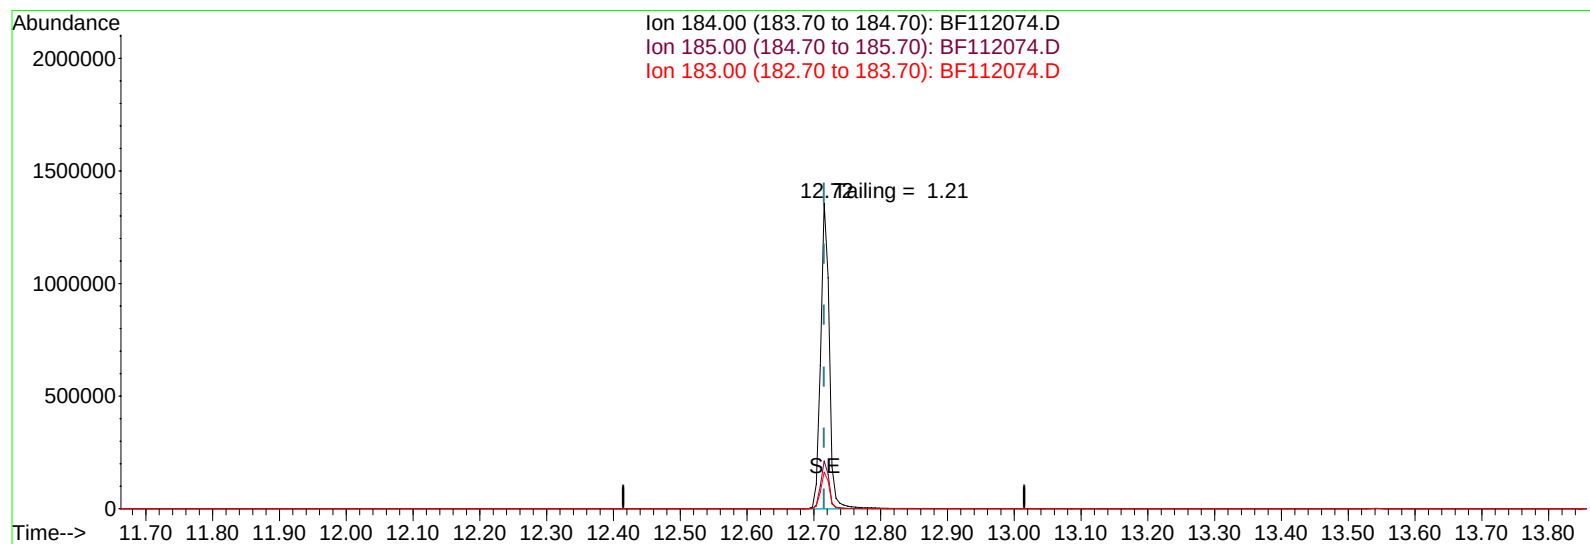

(77) Benzidine

12.715min (+0.000) 34747.24ng

response 1228905

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	15.64
183.00	12.50	11.98
0.00	0.00	0.00