
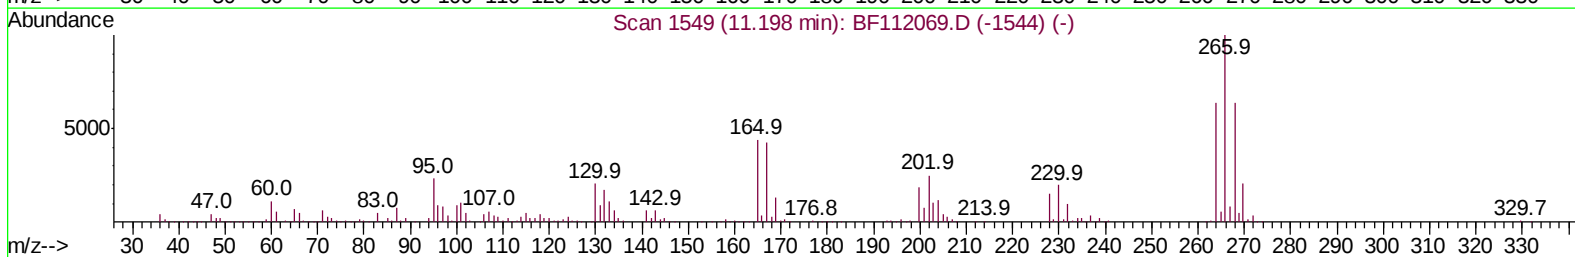
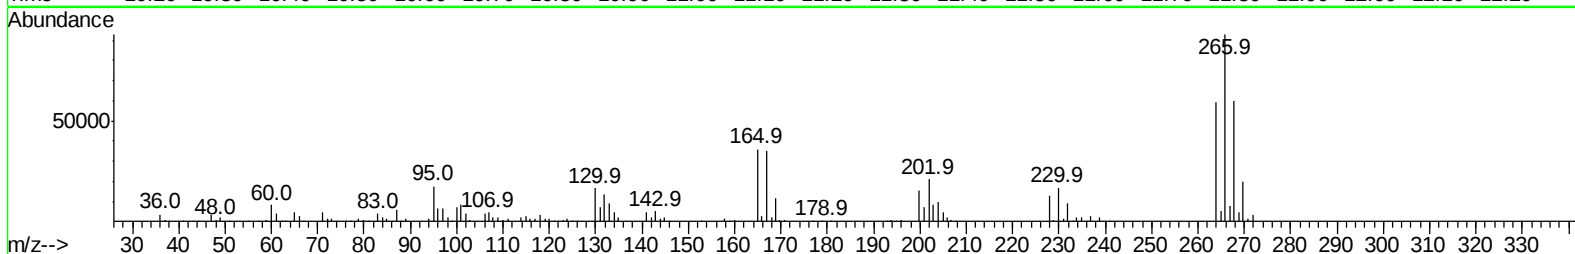


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011719\
Data File : BF112099.D
Acq On : 17 Jan 2019 20:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 03:57:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 16 18:22:05 2019
Response via : Initial Calibration

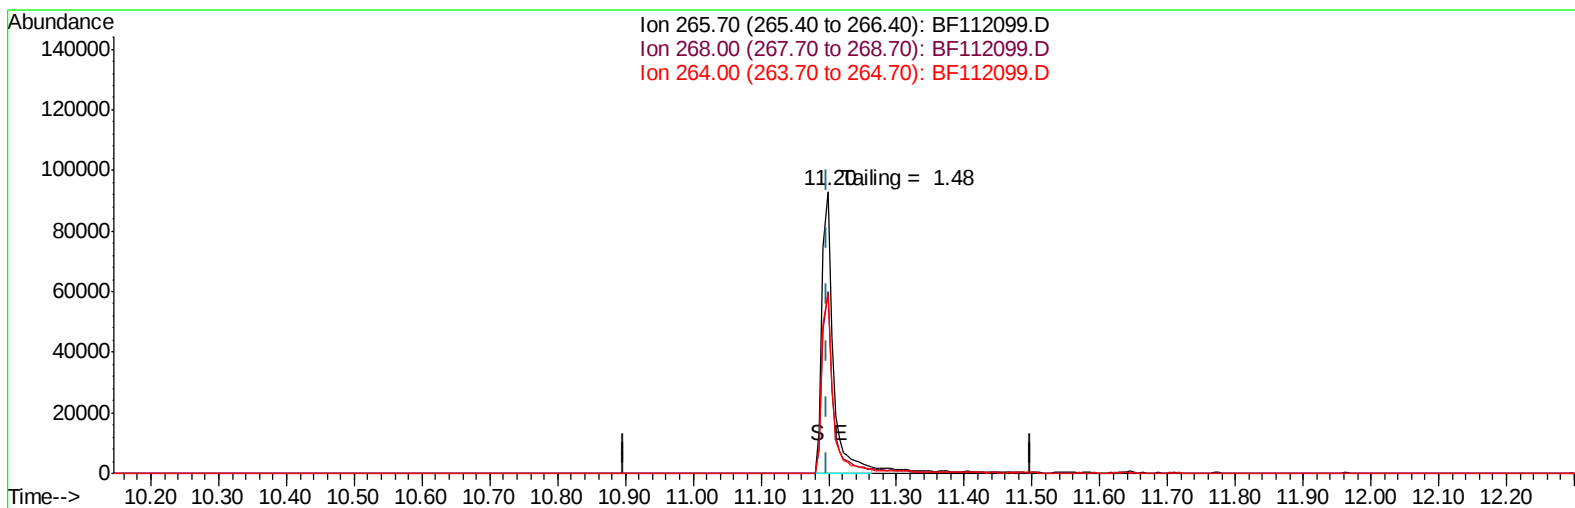

TIC: BF112099.D

(70) Pentachlorophenol (C)




11.198min (+0.000) 43756.86ng

response 106001

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.52
264.00	63.60	63.78
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011719\
Data File : BF112099.D
Acq On : 17 Jan 2019 20:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 03:57:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 16 18:22:05 2019
Response via : Initial Calibration

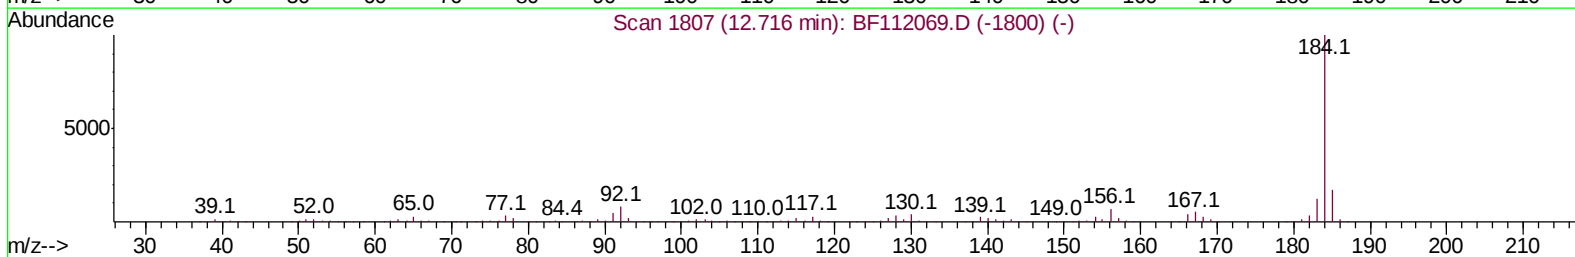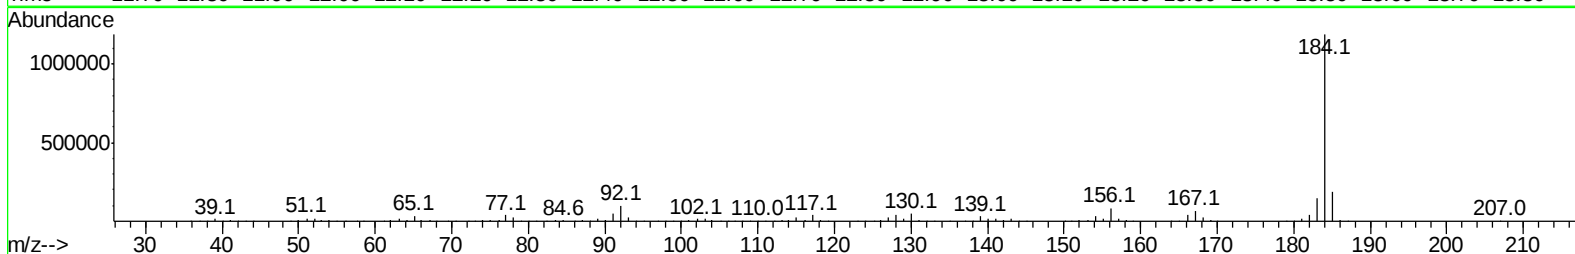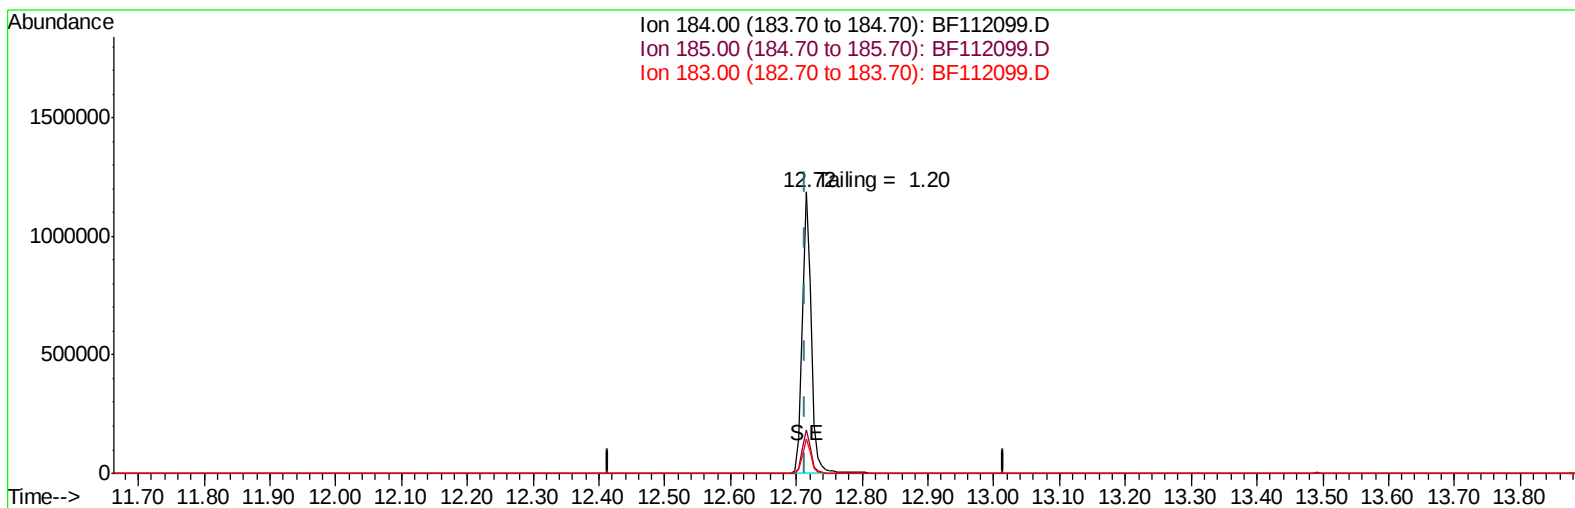

TIC: BF112099.D

(77) Benzidine

12.716min (+0.001) 314550.96ng

response 1133462

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	15.52
183.00	12.50	12.13
0.00	0.00	0.00