


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011719\
 Data File : BF112074.D
 Acq On : 17 Jan 2019 8:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 16 18:22:05 2019

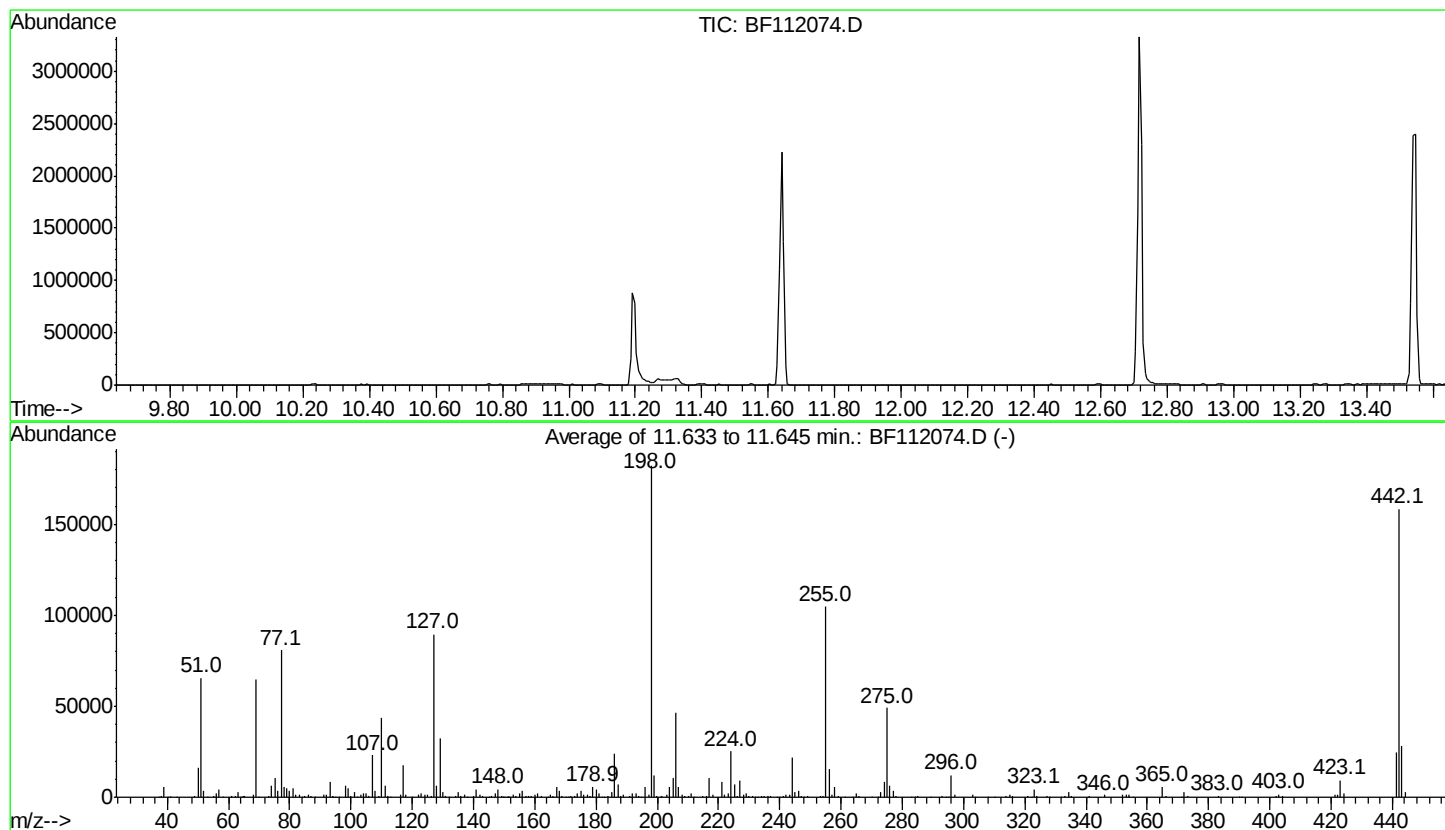

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	65765	PASS
68	69	0.00	2	1.7	1091	PASS
69	198	0.00	100	35.7	65097	PASS
70	69	0.00	2	0.4	265	PASS
127	198	10	80	49.2	89653	PASS
197	198	0.00	2	0.7	1190	PASS
198	198	100	100	100.0	182261	PASS
199	198	5	9	6.7	12168	PASS
275	198	10	60	26.8	48933	PASS
365	198	1	100	3.2	5883	PASS
441	198	0.01	100	13.5	24577	PASS
442	198	50	100	86.9	158432	PASS
443	442	15	24	17.9	28347	PASS