


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011719\
 Data File : BF112099.D
 Acq On : 17 Jan 2019 20:36
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 16 18:22:05 2019

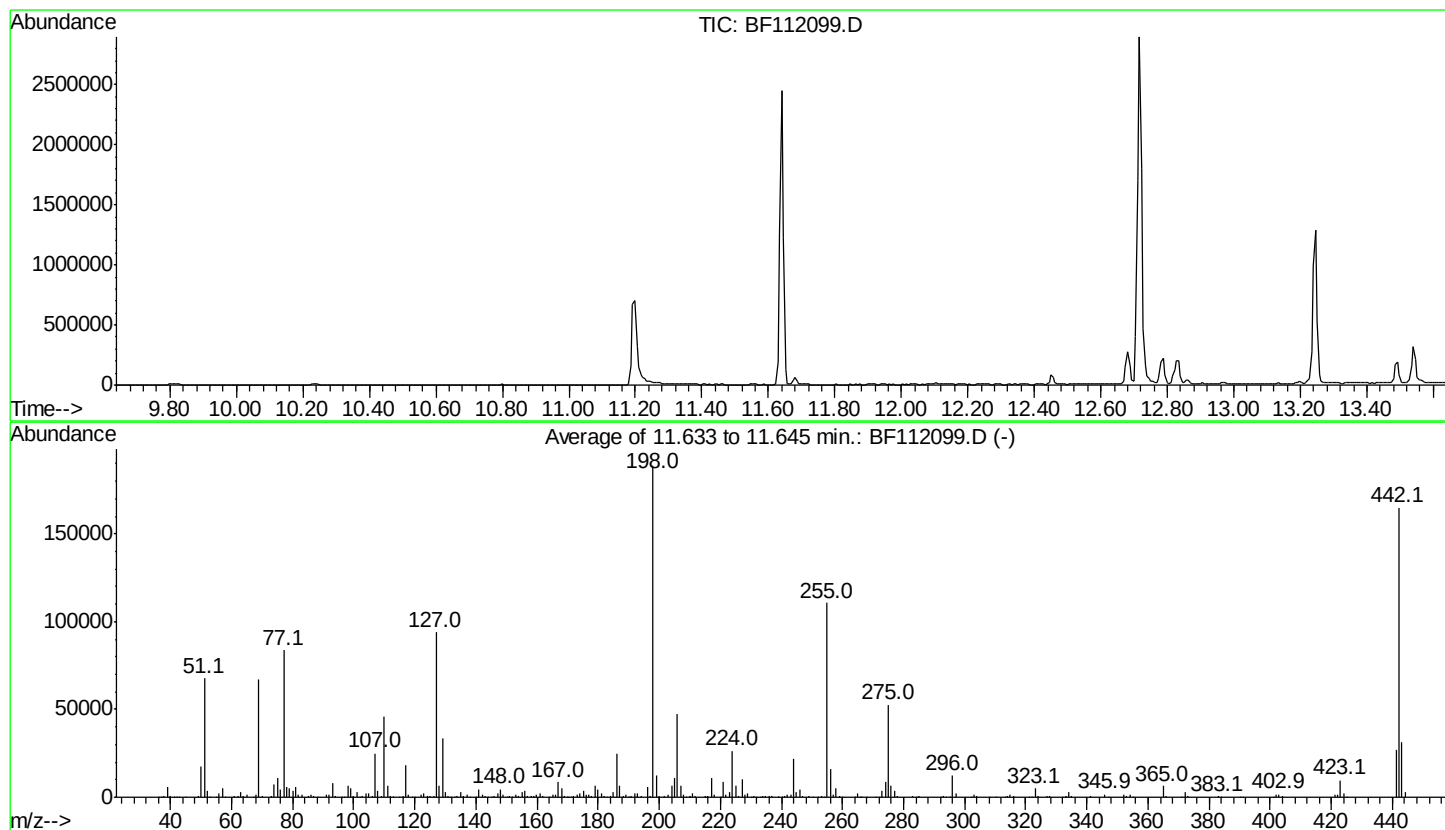

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	67624	PASS
68	69	0.00	2	1.9	1247	PASS
69	198	0.00	100	35.4	66840	PASS
70	69	0.00	2	0.6	429	PASS
127	198	10	80	49.7	93829	PASS
197	198	0.00	2	0.3	504	PASS
198	198	100	100	100.0	188842	PASS
199	198	5	9	6.7	12703	PASS
275	198	10	60	27.9	52752	PASS
365	198	1	100	3.4	6384	PASS
441	198	0.01	100	14.2	26776	PASS
442	198	50	100	87.4	165098	PASS
443	442	15	24	18.9	31185	PASS