
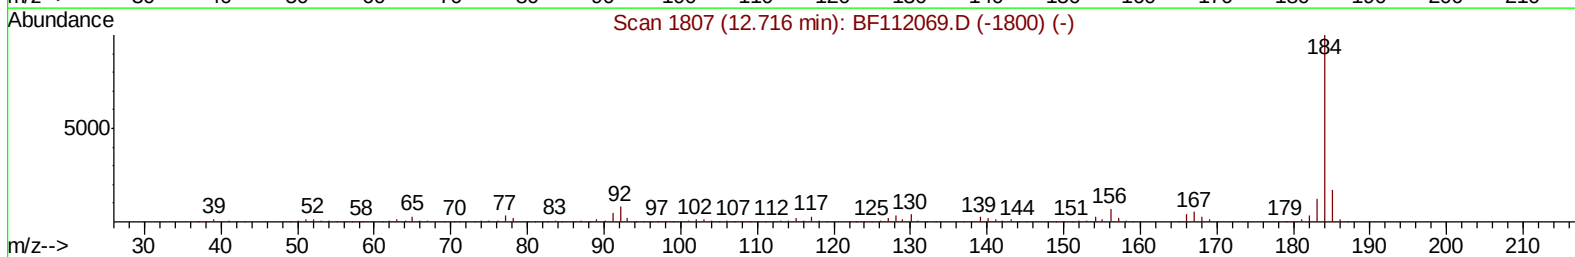
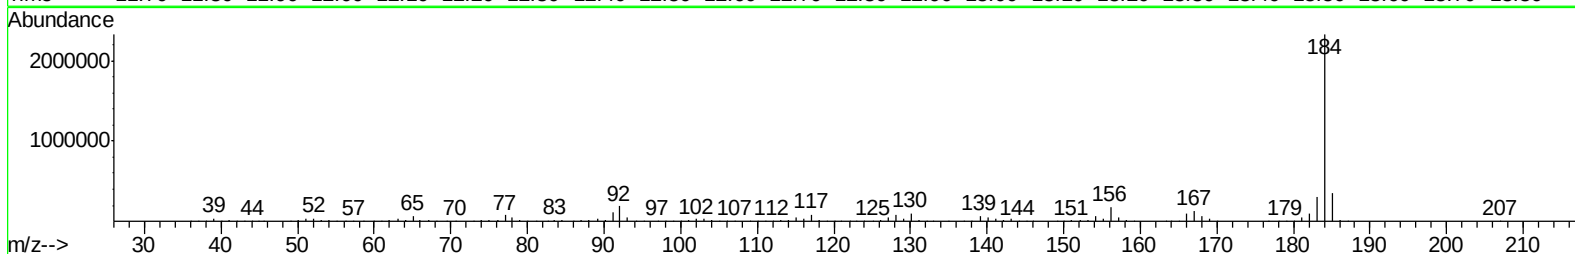


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF011819\  
Data File : BF112125.D  
Acq On : 18 Jan 2019 15:32  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 05:50:45 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF011619.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jan 19 01:02:12 2019  
Response via : Initial Calibration

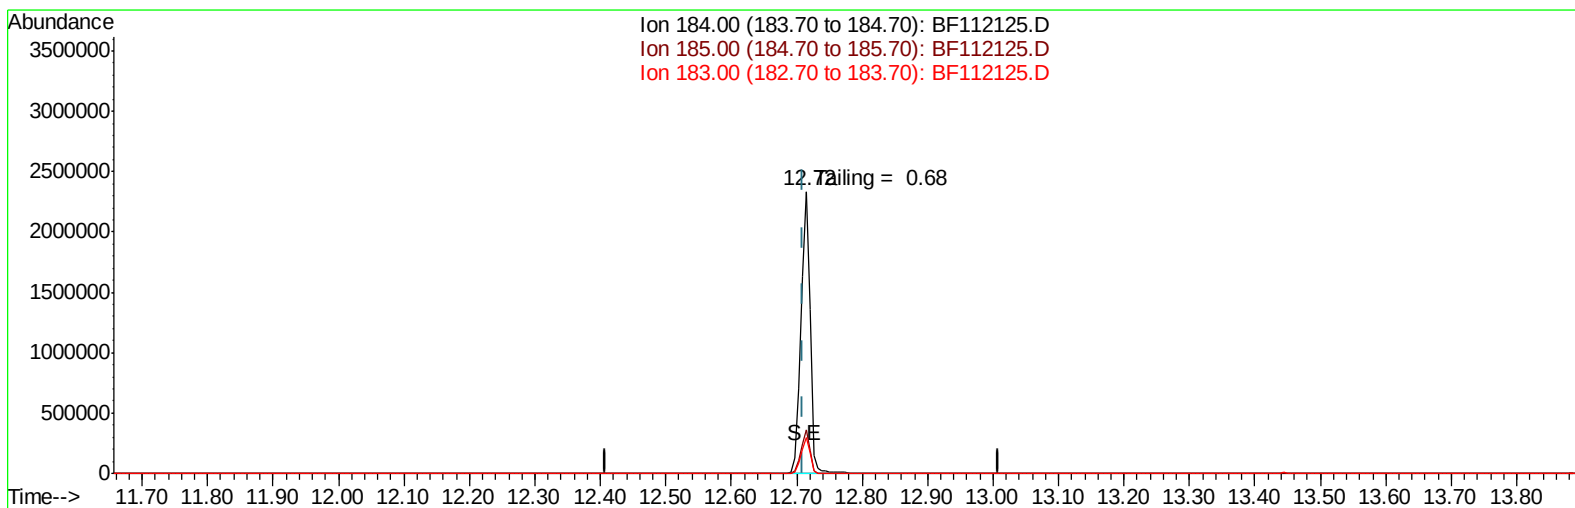

TIC: BF112125.D

(77) Benzidine




12.716min (+0.006) 127196.07ng

response 2287466

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 17.40 | 15.41 |
| 183.00 | 12.50 | 12.81 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF011819\  
Data File : BF112125.D  
Acq On : 18 Jan 2019 15:32  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 05:50:45 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF011619.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jan 19 01:02:12 2019  
Response via : Initial Calibration

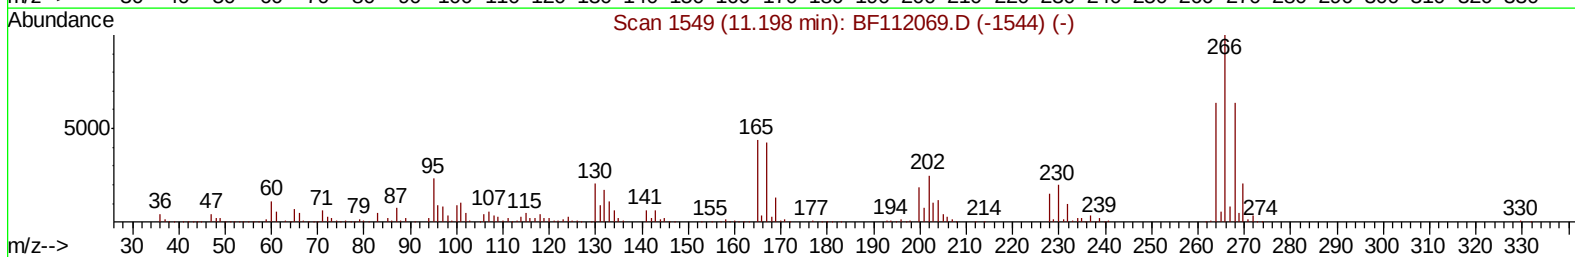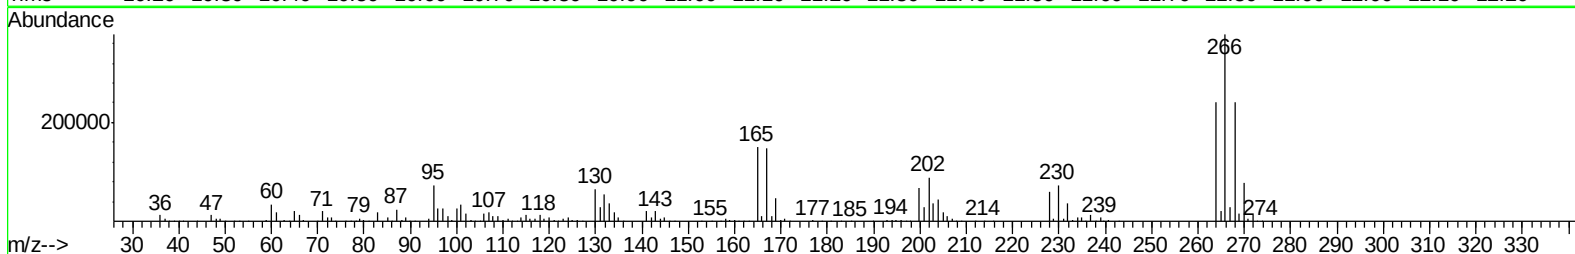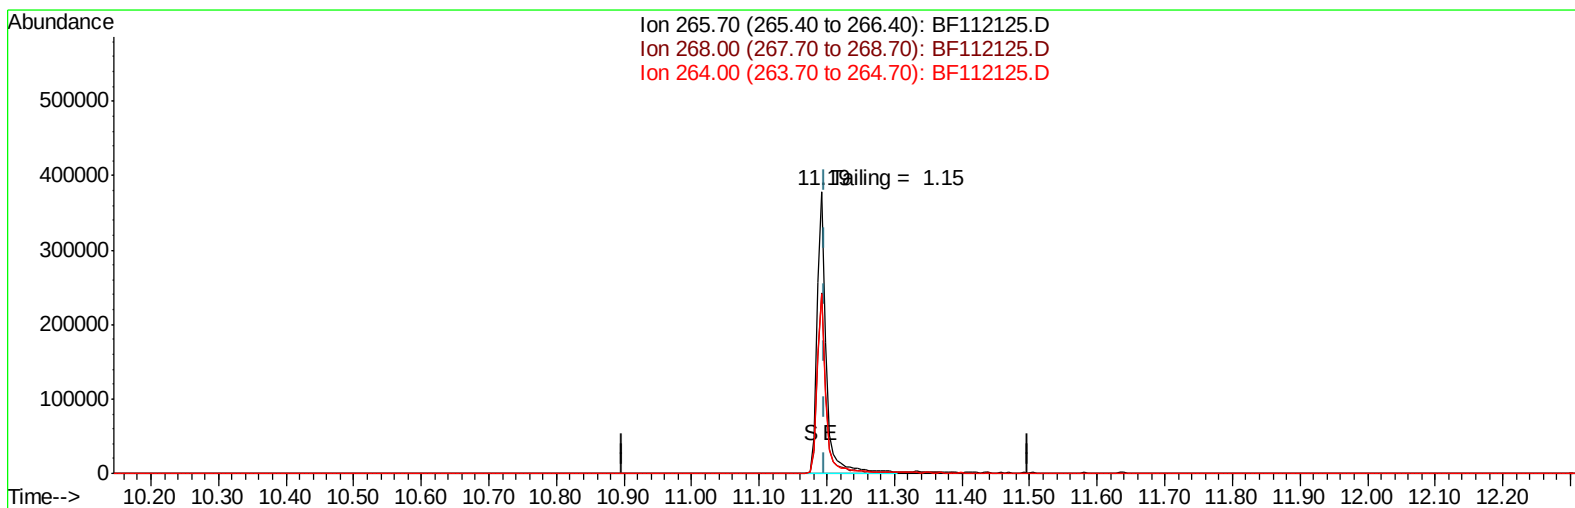

TIC: BF112125.D

(70) Pentachlorophenol (C)

11.192min (-0.006) 121911.00ng

response 365225

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.00 | 63.97 |
| 264.00 | 63.60 | 63.76 |
| 0.00   | 0.00  | 0.00  |