


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011819\
 Data File : BF112125.D
 Acq On : 18 Jan 2019 15:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 23:33:58 2019

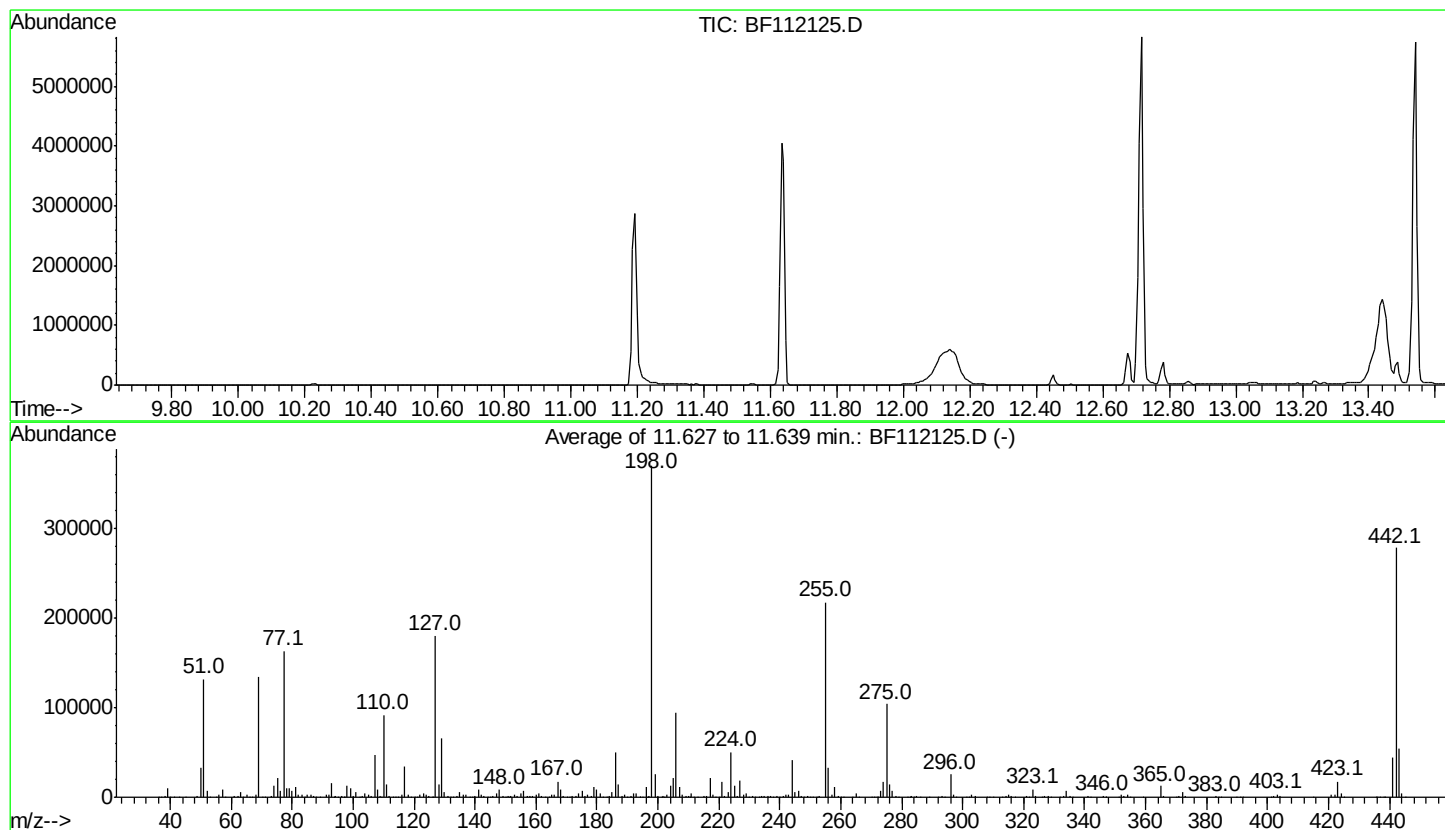

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	131264	PASS
68	69	0.00	2	2.0	2702	PASS
69	198	0.00	100	36.1	133416	PASS
70	69	0.00	2	0.5	710	PASS
127	198	10	80	48.7	179850	PASS
197	198	0.00	2	0.5	1824	PASS
198	198	100	100	100.0	369386	PASS
199	198	5	9	6.9	25470	PASS
275	198	10	60	28.1	103834	PASS
365	198	1	100	3.3	12198	PASS
441	198	0.01	100	11.8	43691	PASS
442	198	50	100	75.2	277752	PASS
443	442	15	24	19.7	54633	PASS