
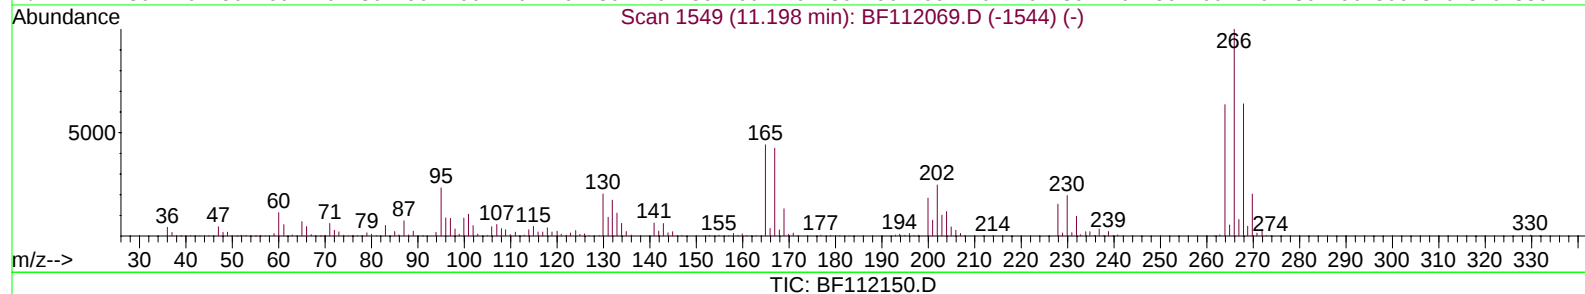
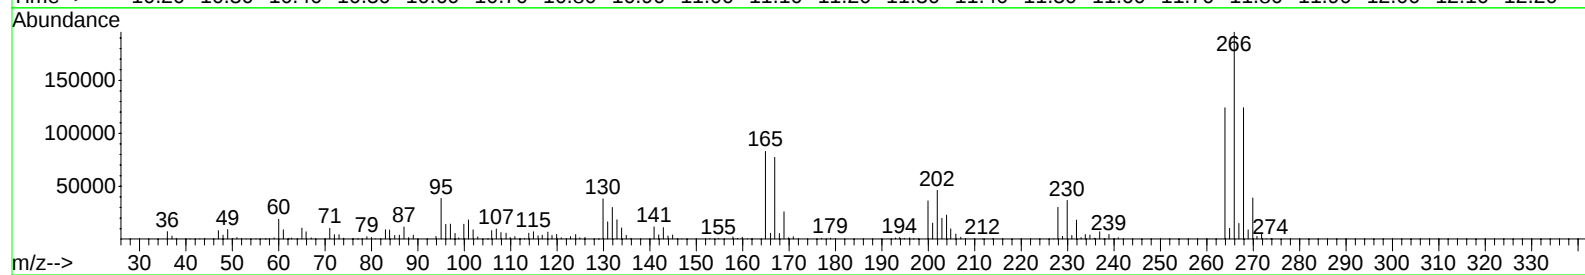


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012119\  
Data File   : BF112150.D  
Acq On      : 21 Jan 2019   11:12  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jan 21 13:39:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 19 01:02:12 2019
Response via : Initial Calibration

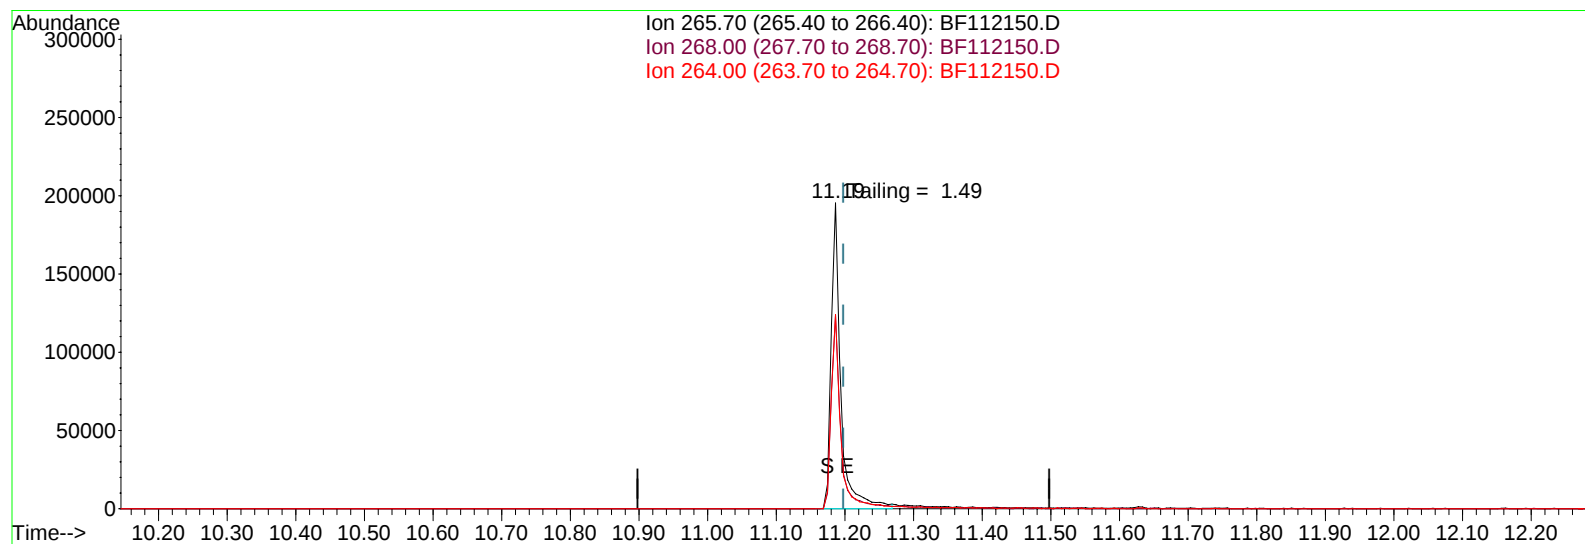

(70) Pentachlorophenol (C)




11.186min (-0.012) 221555.90ng

response 193356

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.50
264.00	63.60	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012119\
 Data File : BF112150.D
 Acq On : 21 Jan 2019 11:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 13:39:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 19 01:02:12 2019
 Response via : Initial Calibration

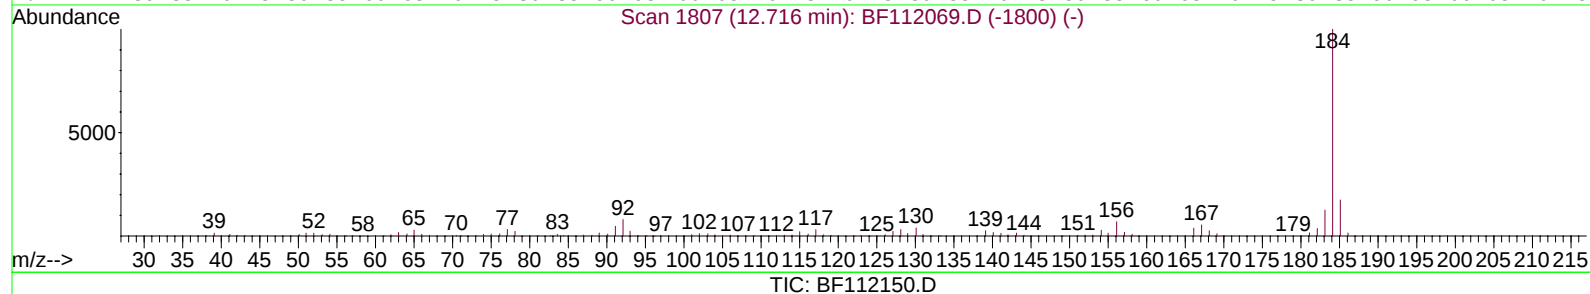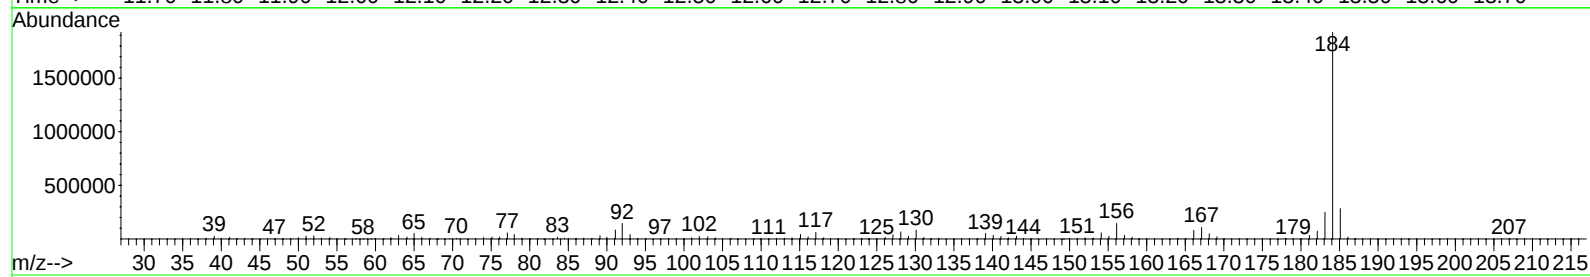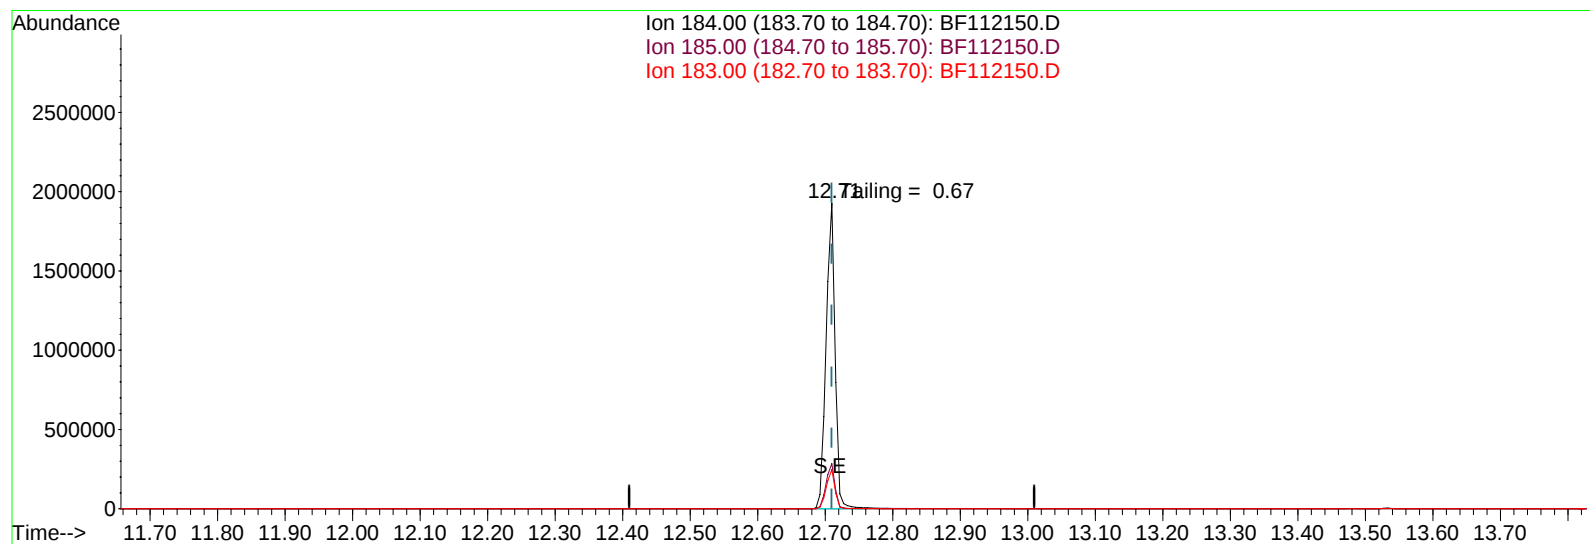

(77) Benzidine

12.710min (+0.000) 67682.68ng

response 1784008

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.75
183.00	12.50	12.84
0.00	0.00	0.00