
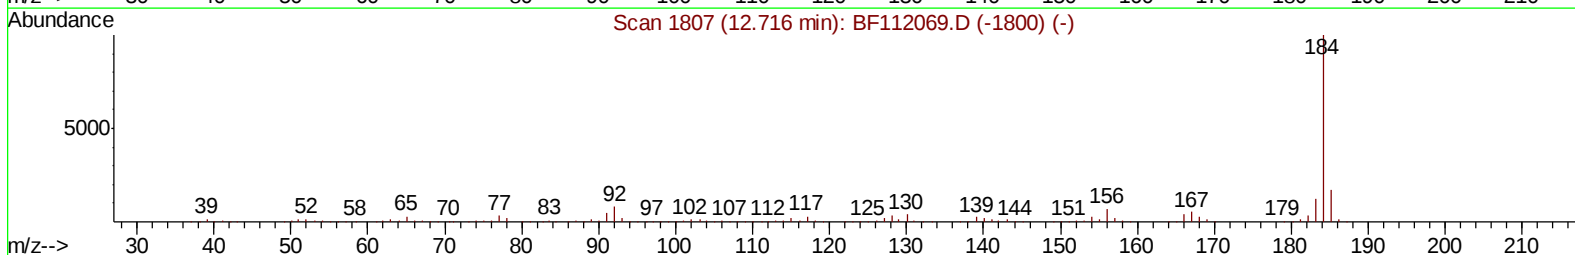
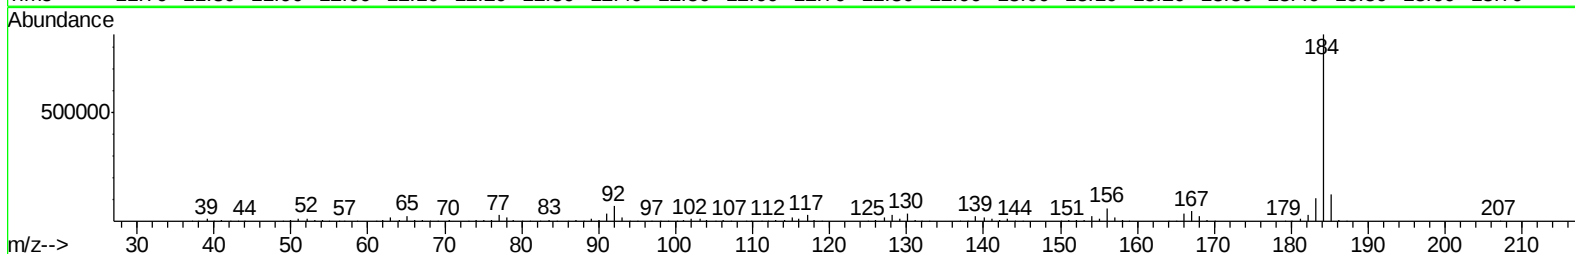


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012119\
Data File : BF112173.D
Acq On : 21 Jan 2019 22:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 03:12:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 19 01:02:12 2019
Response via : Initial Calibration

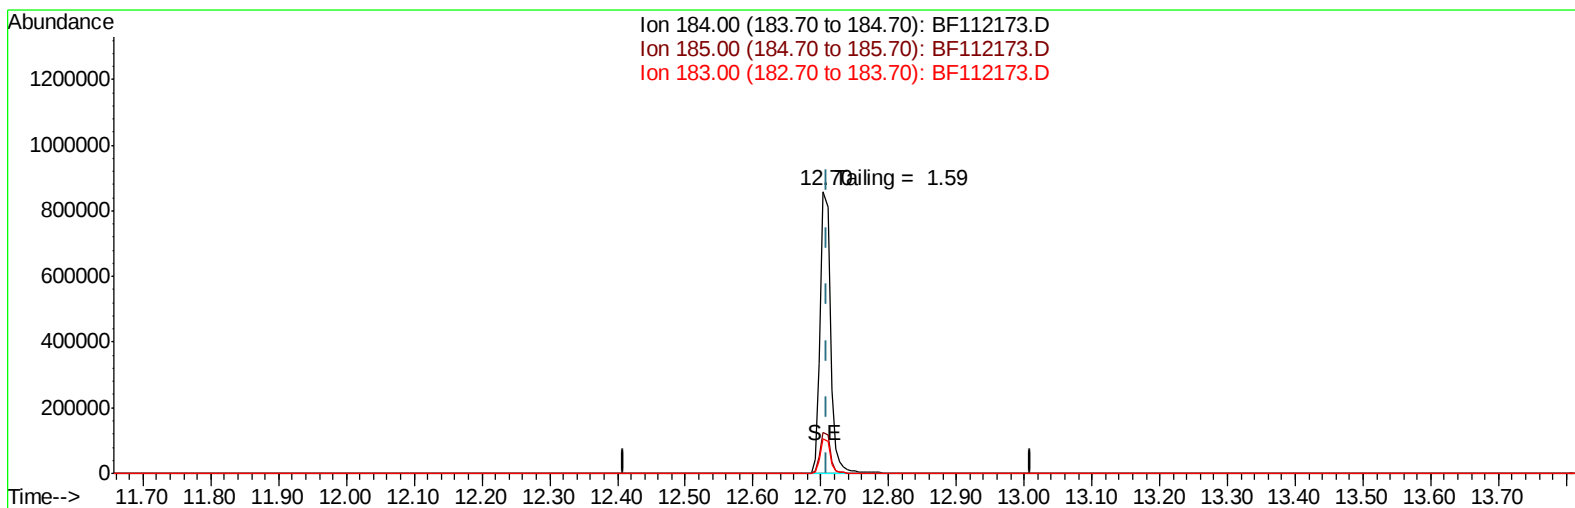

TIC: BF112173.D

(77) Benzidine




12.704min (-0.006) 205738.81ng

response 878655

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.54
183.00	12.50	12.24
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012119\
Data File : BF112173.D
Acq On : 21 Jan 2019 22:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 03:12:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 19 01:02:12 2019
Response via : Initial Calibration

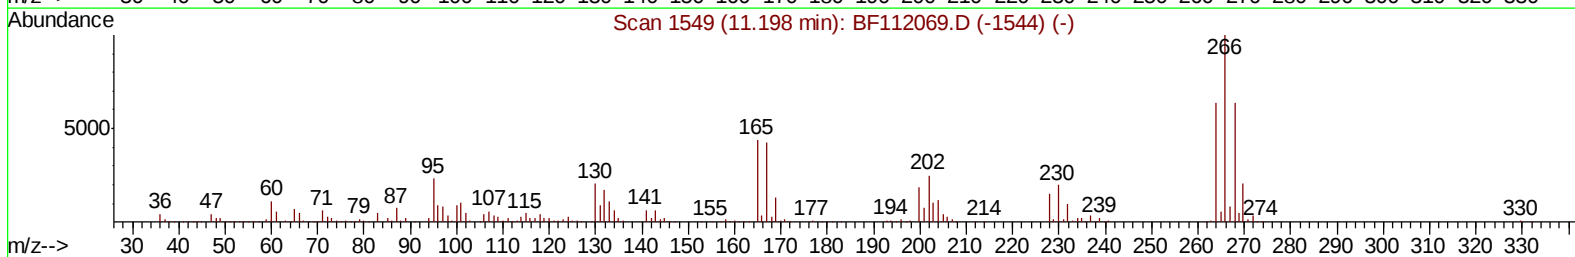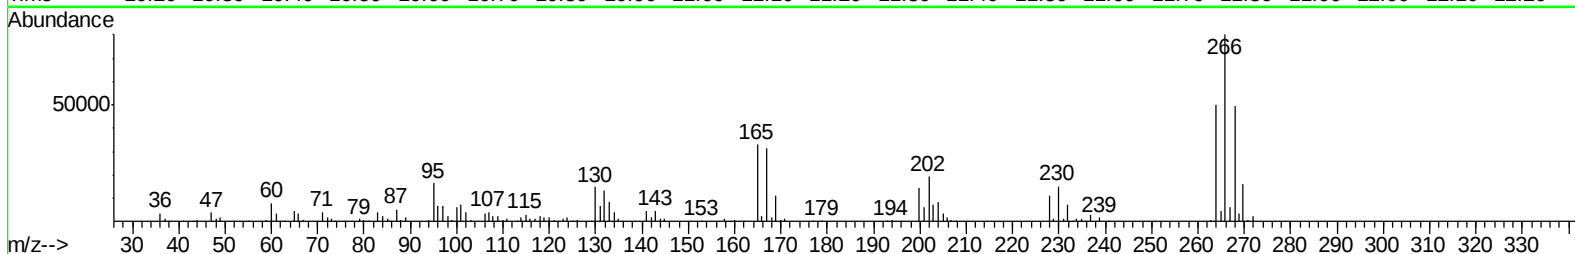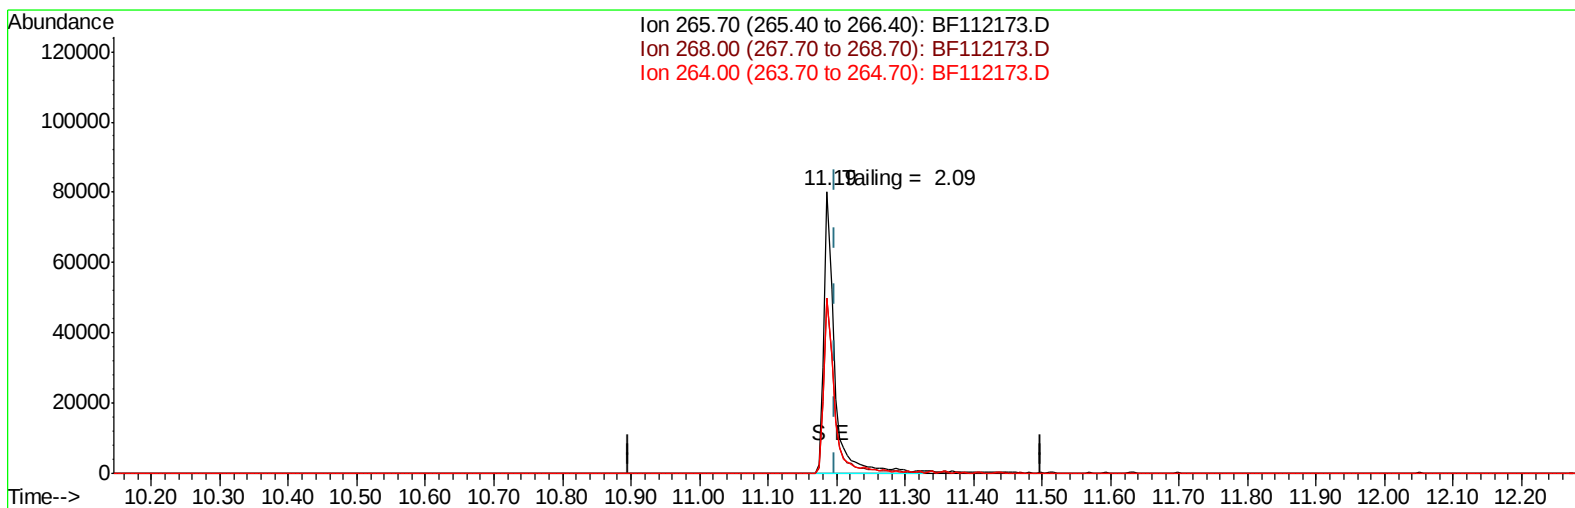

TIC: BF112173.D

(70) Pentachlorophenol (C)

11.186min (-0.012) 116751.65ng

response 81359

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.06
264.00	63.60	62.31
0.00	0.00	0.00