


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012119\
 Data File : BF112150.D
 Acq On : 21 Jan 2019 11:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 19 01:02:12 2019

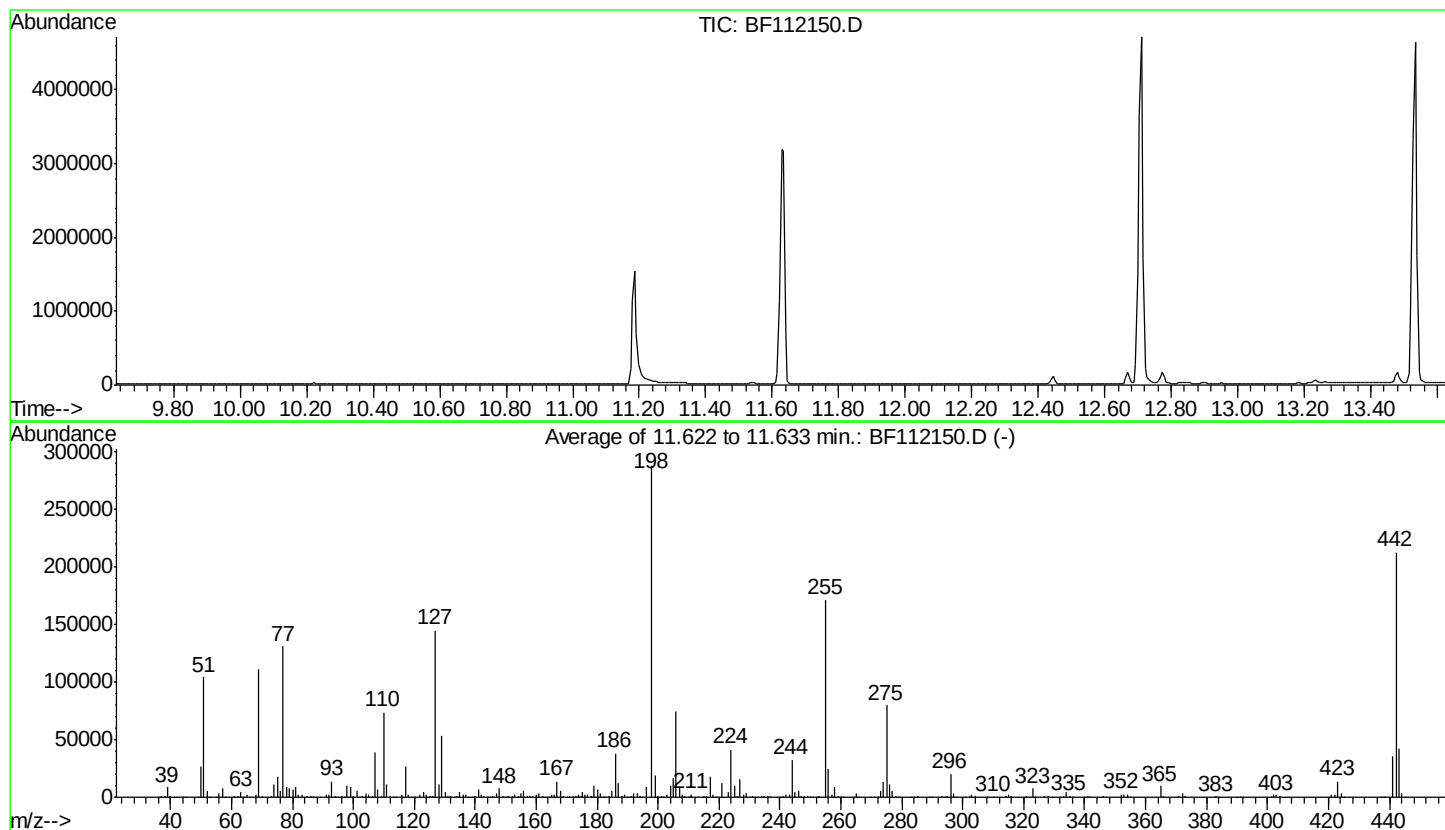

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	104106	PASS
68	69	0.00	2	1.8	2060	PASS
69	198	0.00	100	38.7	111410	PASS
70	69	0.00	2	0.6	657	PASS
127	198	10	80	50.3	144680	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	287837	PASS
199	198	5	9	6.7	19226	PASS
275	198	10	60	27.7	79776	PASS
365	198	1	100	3.3	9616	PASS
441	198	0.01	100	12.3	35521	PASS
442	198	50	100	73.8	212458	PASS
443	442	15	24	20.0	42386	PASS