
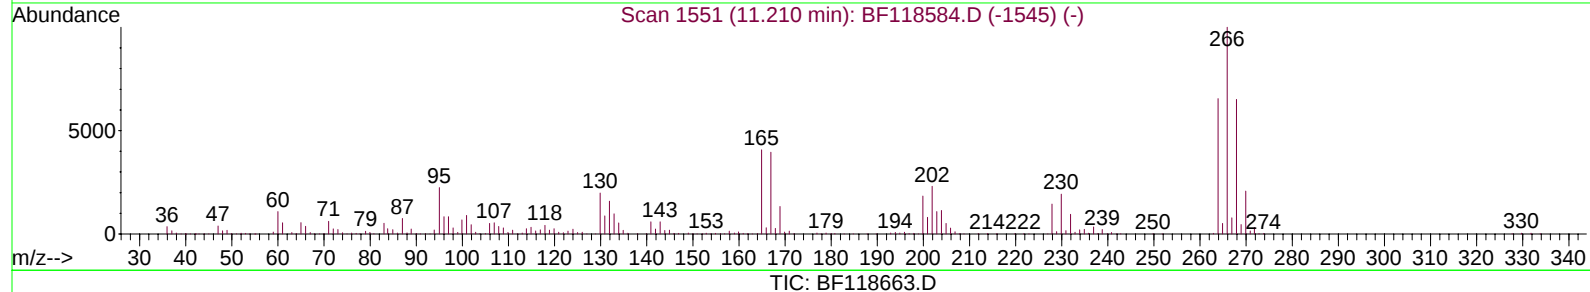
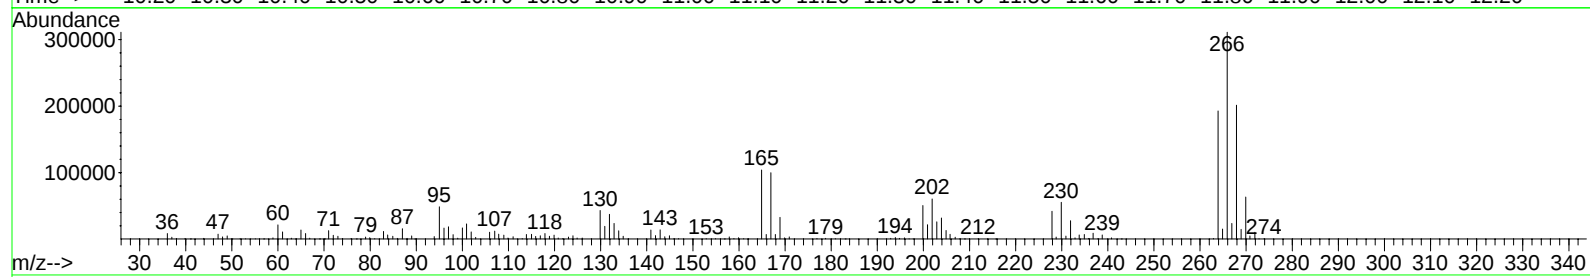


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012220\
 Data File : BF118663.D
 Acq On : 22 Jan 2020 14:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 18:33:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 20 14:45:03 2020
 Response via : Initial Calibration

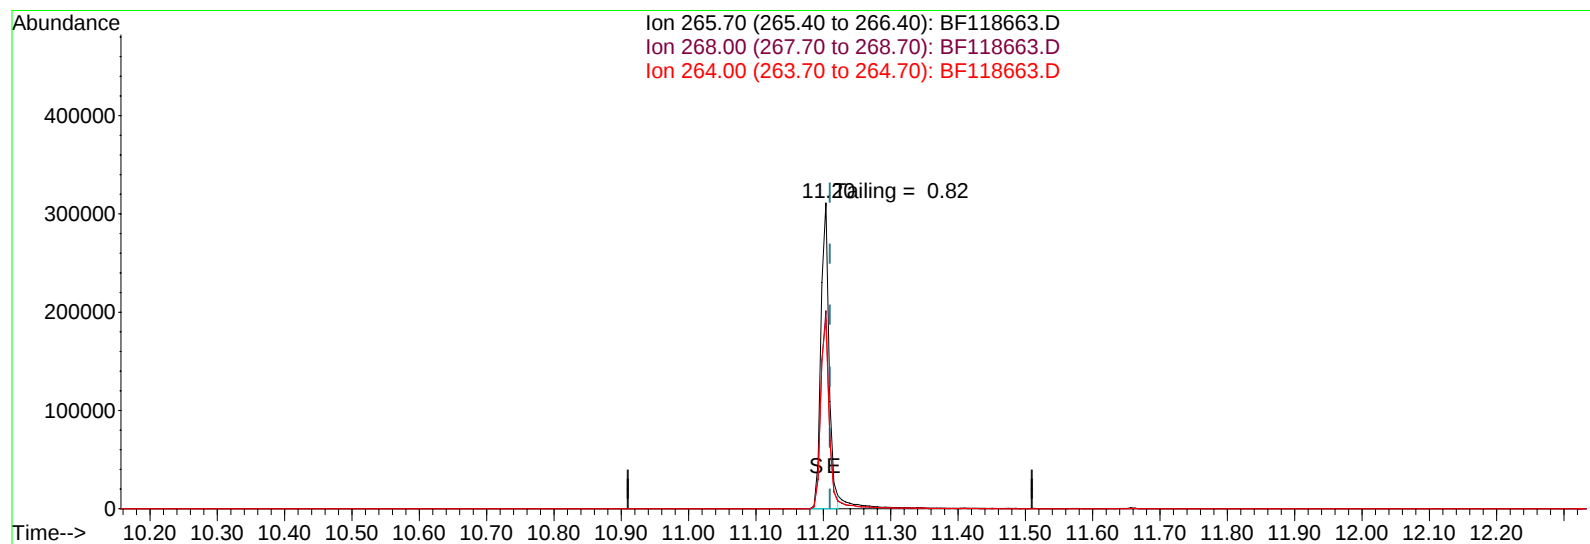

(70) Pentachlorophenol (C)




11.204min (-0.006) 38038.00ng

response 280526

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.72
264.00	65.50	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012220\
 Data File : BF118663.D
 Acq On : 22 Jan 2020 14:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 18:33:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 20 14:45:03 2020
 Response via : Initial Calibration

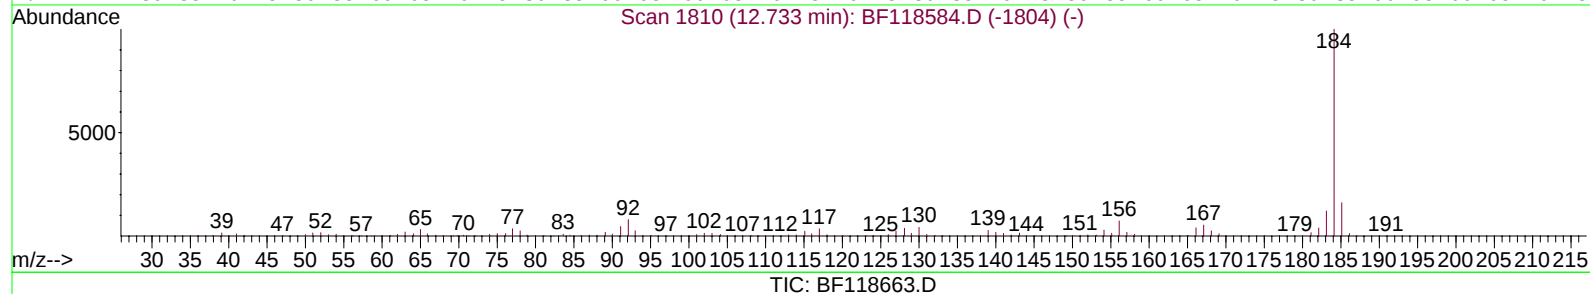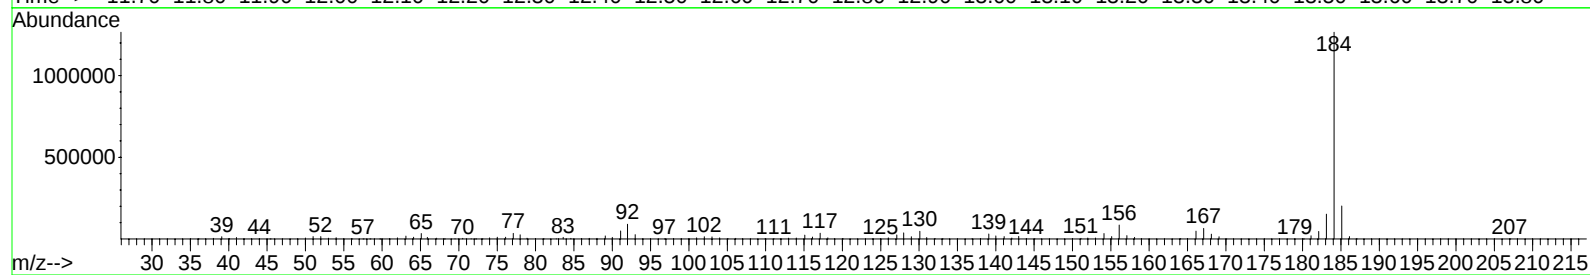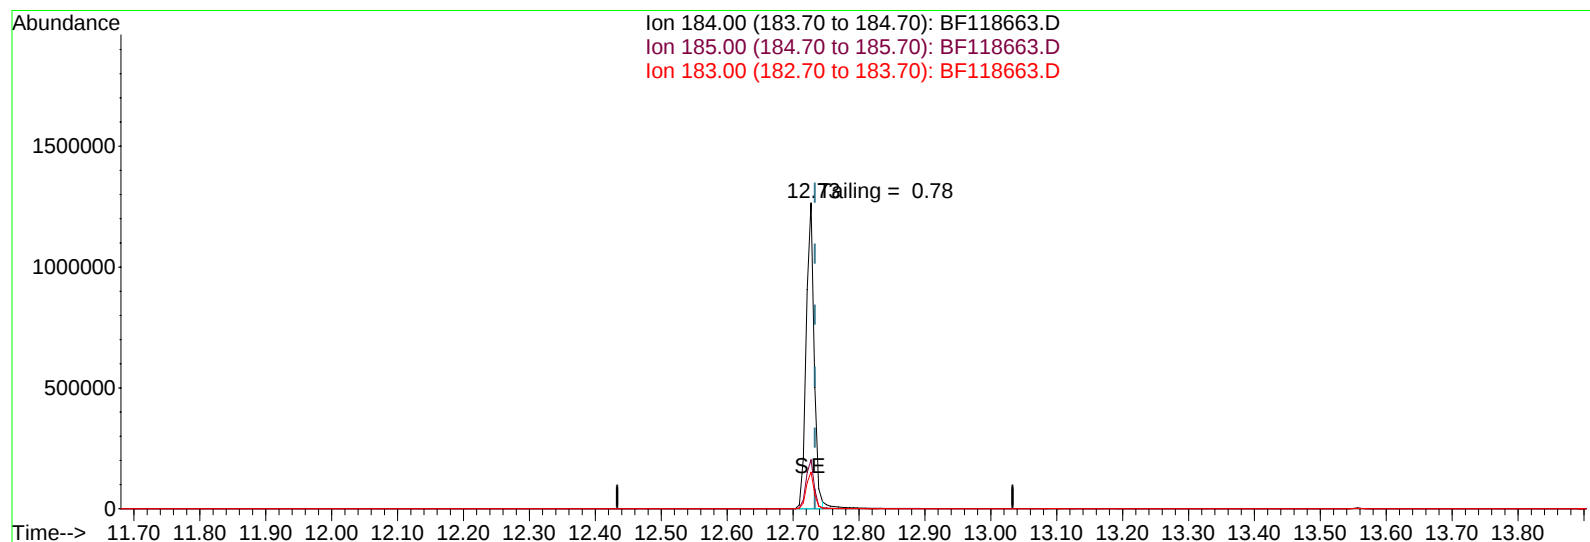

(77) Benzidine

12.727min (-0.006) 0.00ng

response 1096345

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	16.01
183.00	12.00	11.99
0.00	0.00	0.00