


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012220\
 Data File : BF118663.D
 Acq On : 22 Jan 2020 14:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 20 14:45:03 2020

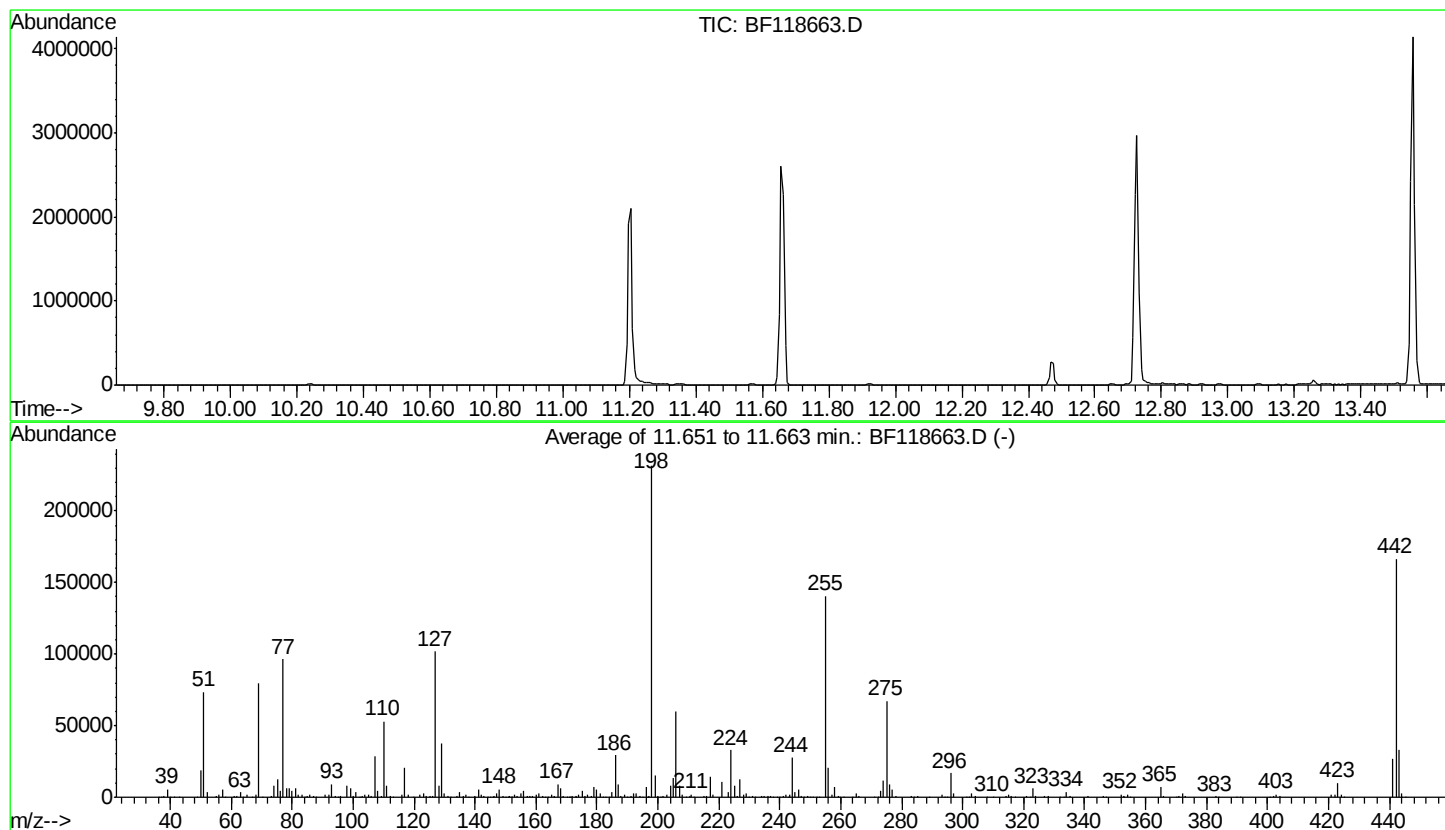

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	73794	PASS
68	69	0.00	2	1.8	1401	PASS
69	198	0.00	100	34.2	79336	PASS
70	69	0.00	2	0.6	438	PASS
127	198	10	80	43.9	101744	PASS
197	198	0.00	2	0.2	513	PASS
198	198	100	100	100.0	231674	PASS
199	198	5	9	6.6	15356	PASS
275	198	10	60	29.0	67245	PASS
365	198	1	100	3.3	7550	PASS
441	198	0.01	100	11.5	26671	PASS
442	198	50	100	71.8	166440	PASS
443	442	15	24	19.8	33014	PASS