
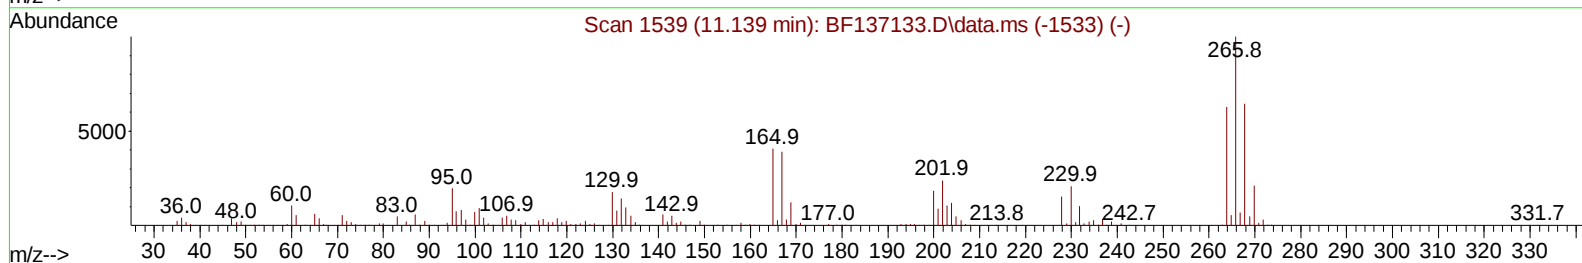
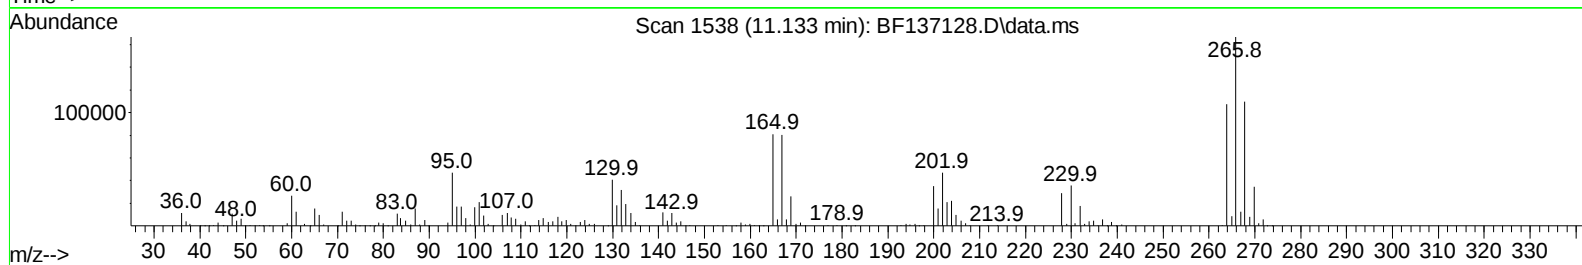


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012324\
Data File : BF137128.D
Acq On : 23 Jan 2024 11:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 16:36:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 15:48:50 2024
Response via : Initial Calibration

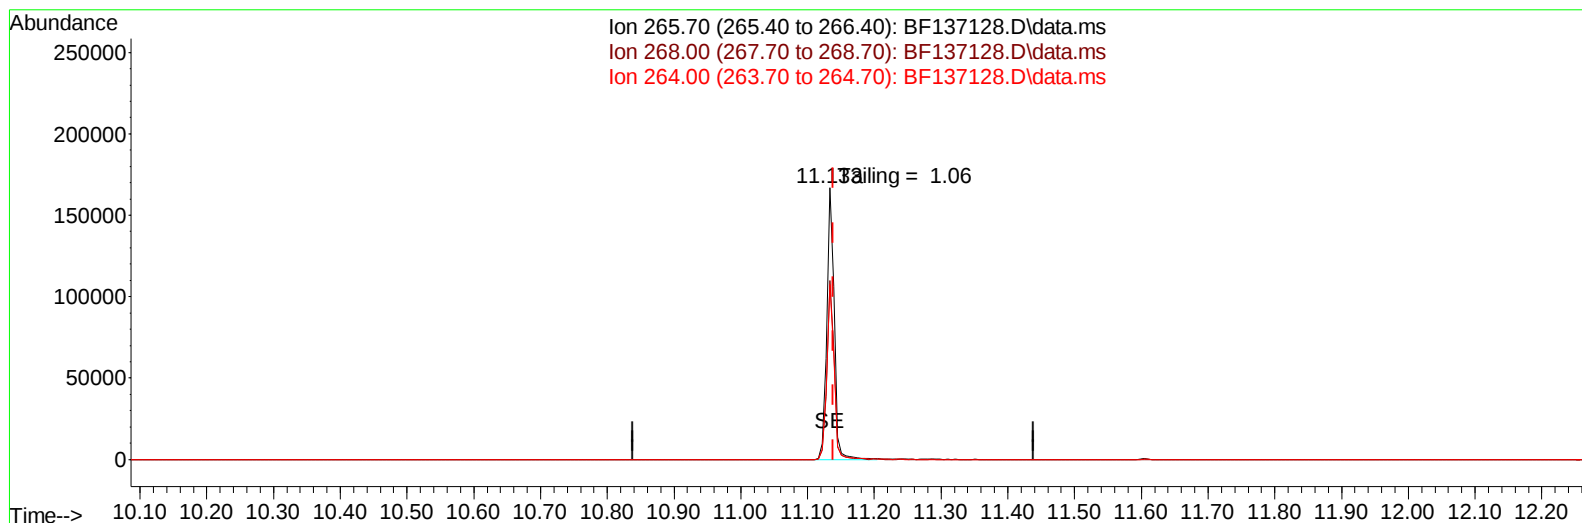




TIC: BF137128.D\data.ms

(70) Pentachlorophenol (C)**11.133min (-0.006) 20512.13 ng****response 131947**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.88
264.00	62.80	64.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012324\
Data File : BF137128.D
Acq On : 23 Jan 2024 11:10
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 16:36:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 15:48:50 2024
Response via : Initial Calibration

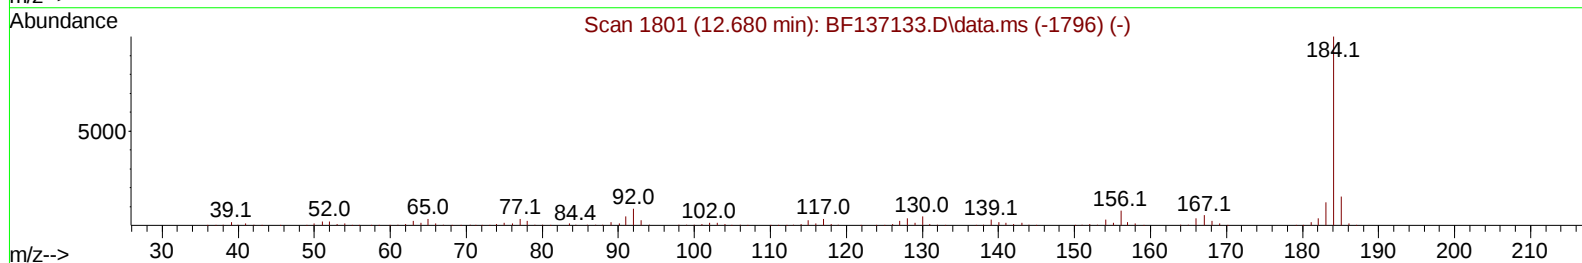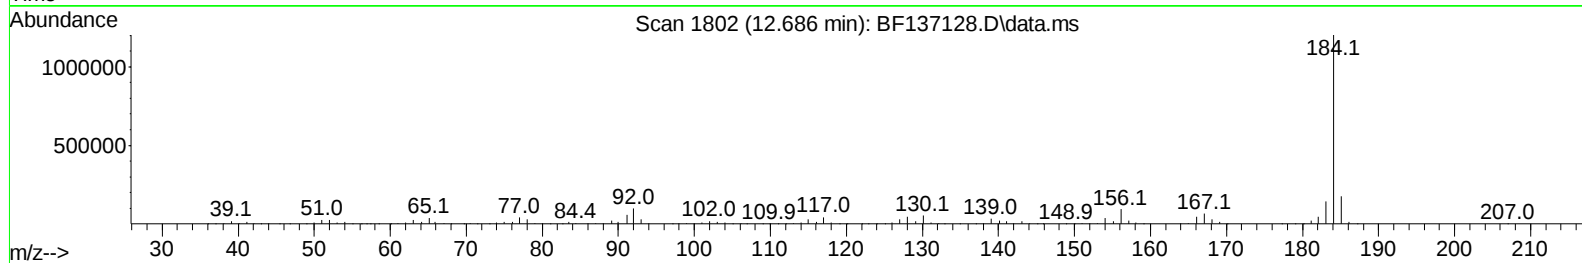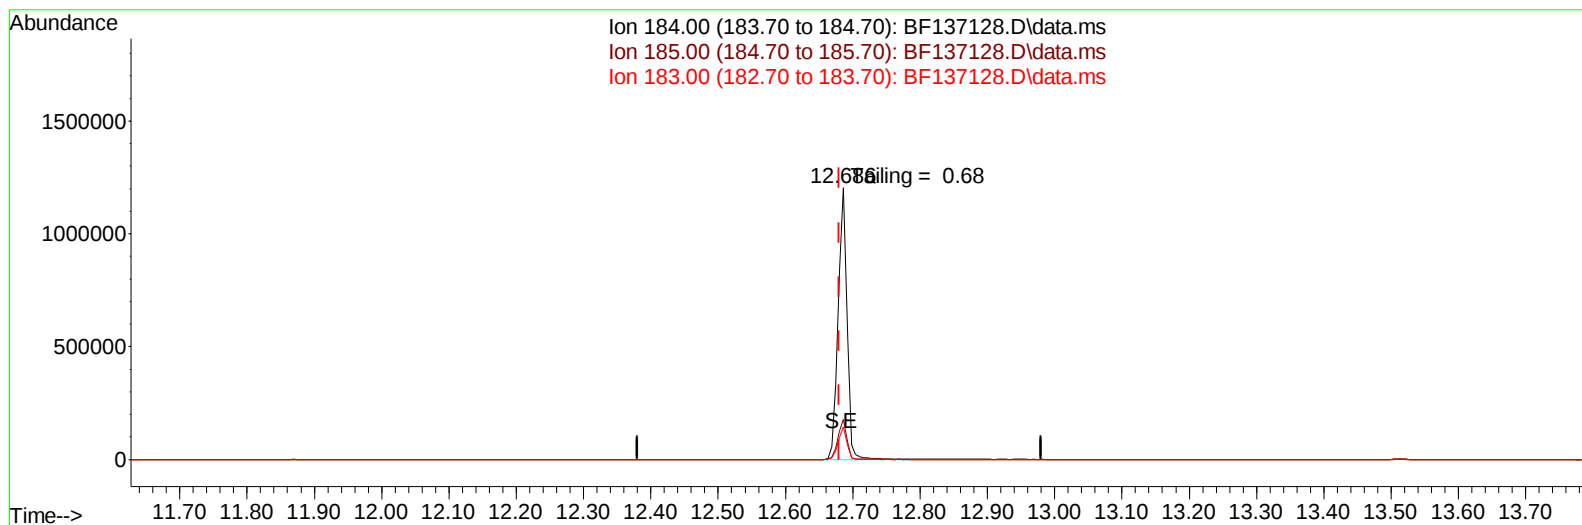

TIC: BF137128.D\data.ms

(77) Benzidine**12.686min (+ 0.006) 0.00 ng****response 1092488**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.67
183.00	12.30	11.89
0.00	0.00	0.00