
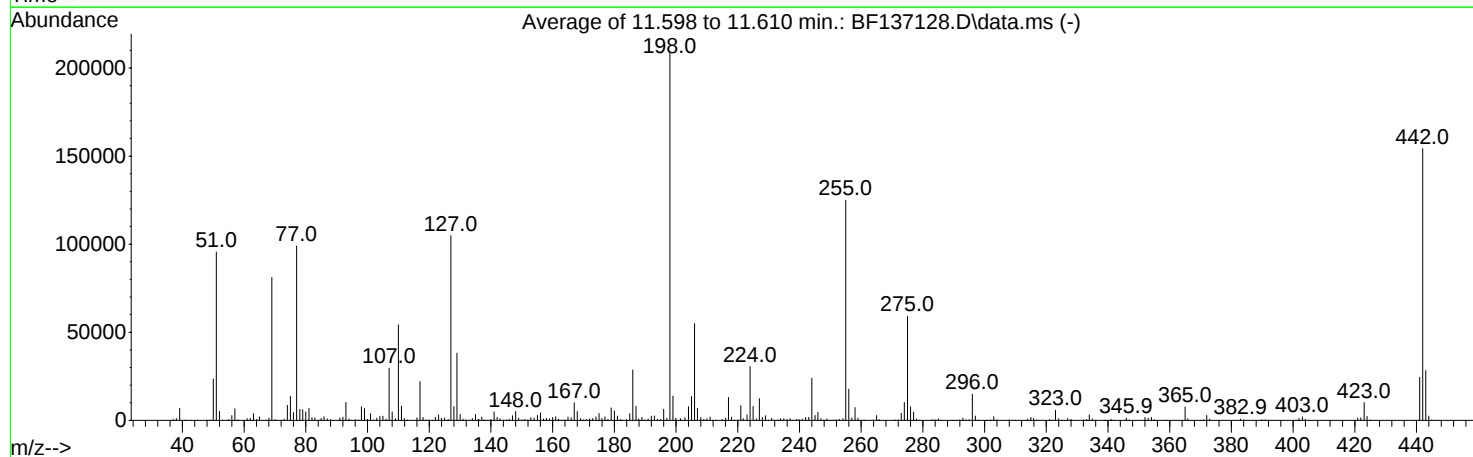


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012324\
Data File : BF137128.D
Acq On : 23 Jan 2024 11:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 24 03:53:23 2024

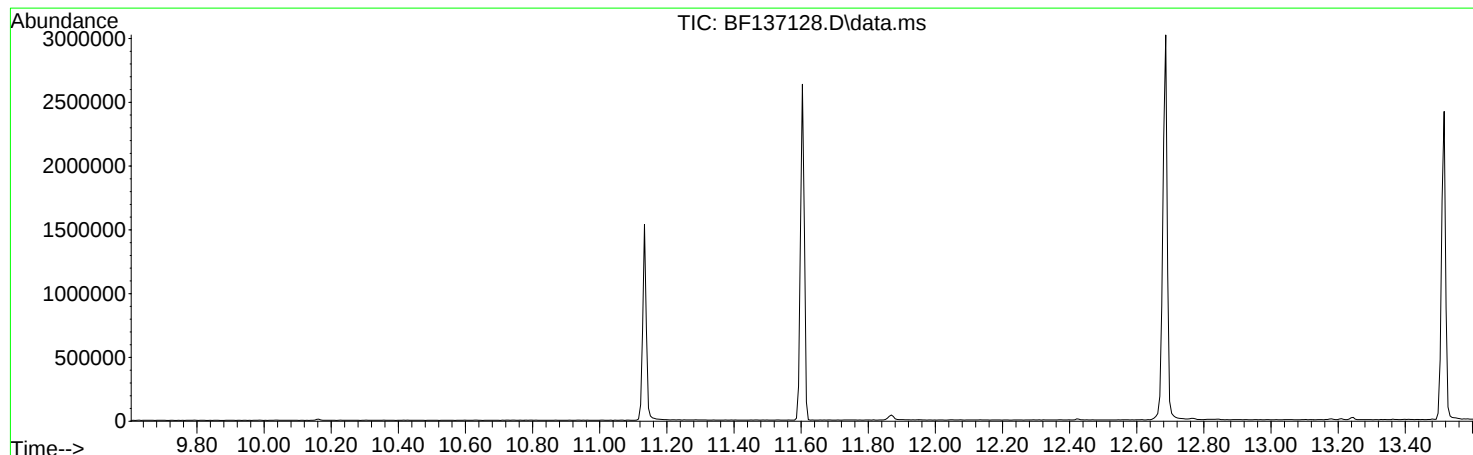




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	95534	PASS
68	69	0.00	2	1.6	1290	PASS
69	198	0.00	100	38.8	81093	PASS
70	69	0.00	2	0.6	498	PASS
127	198	10	80	50.2	104880	PASS
197	198	0.00	2	0.5	1119	PASS
198	198	100	100	100.0	208832	PASS
199	198	5	9	6.6	13836	PASS
275	198	10	60	28.3	59096	PASS
365	198	1	100	3.6	7599	PASS
441	198	0.01	100	11.7	24430	PASS
442	442	50	100	100.0	154211	PASS
443	442	15	24	18.4	28298	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012324\
Data File : BF137128.D
Acq On : 23 Jan 2024 11:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 23 16:36:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 15:48:50 2024
Response via : Initial Calibration

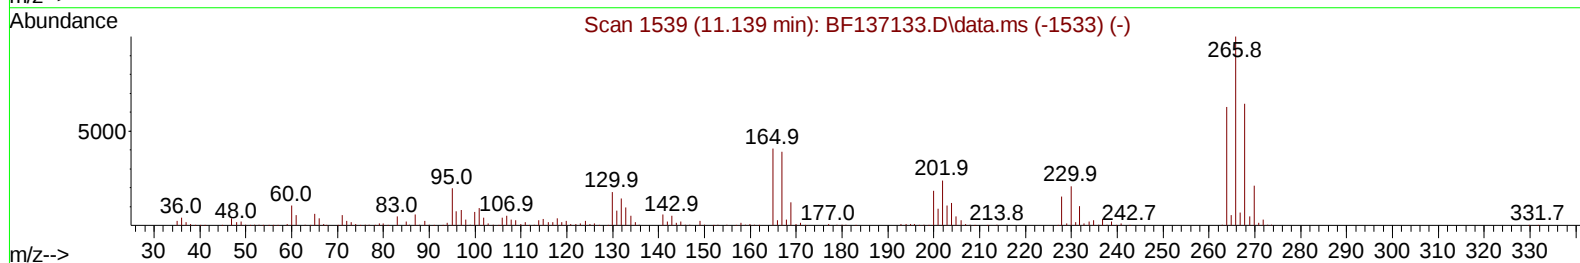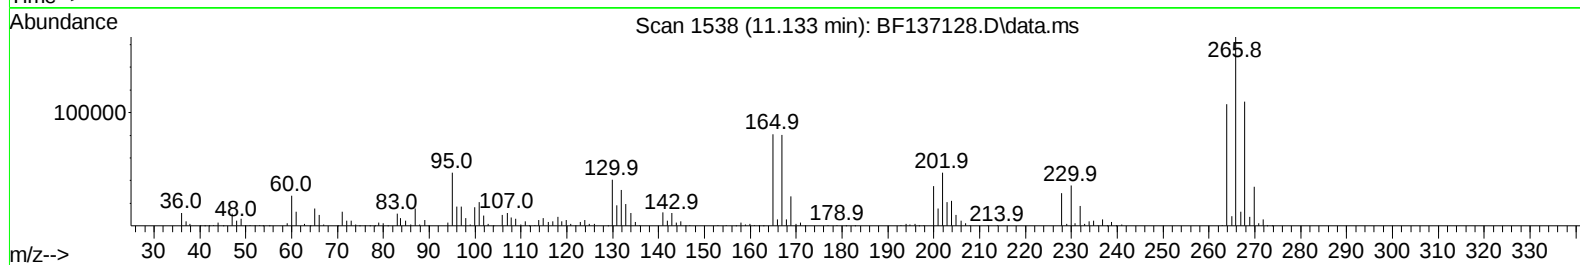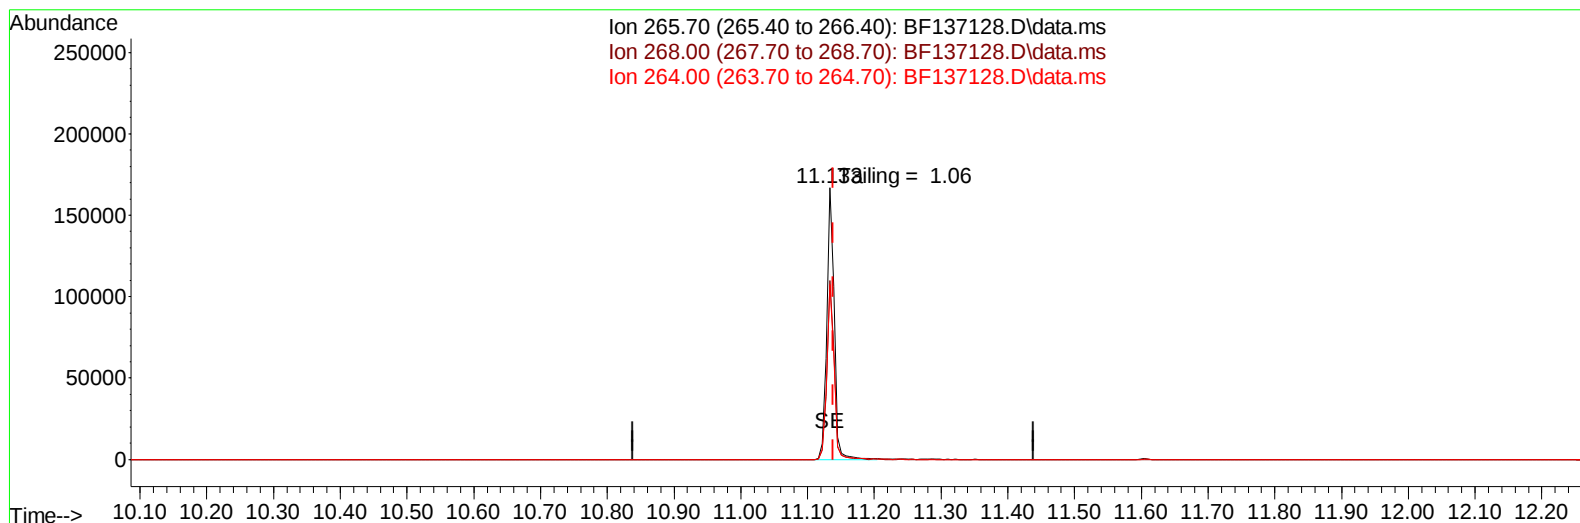

TIC: BF137128.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 20512.13 ng




response 131947

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.88
264.00	62.80	64.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012324\
Data File : BF137128.D
Acq On : 23 Jan 2024 11:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 23 16:36:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 15:48:50 2024
Response via : Initial Calibration

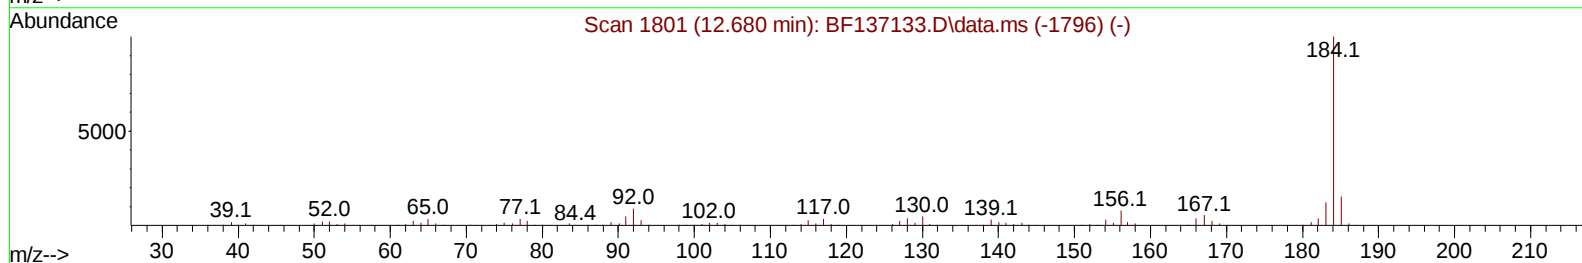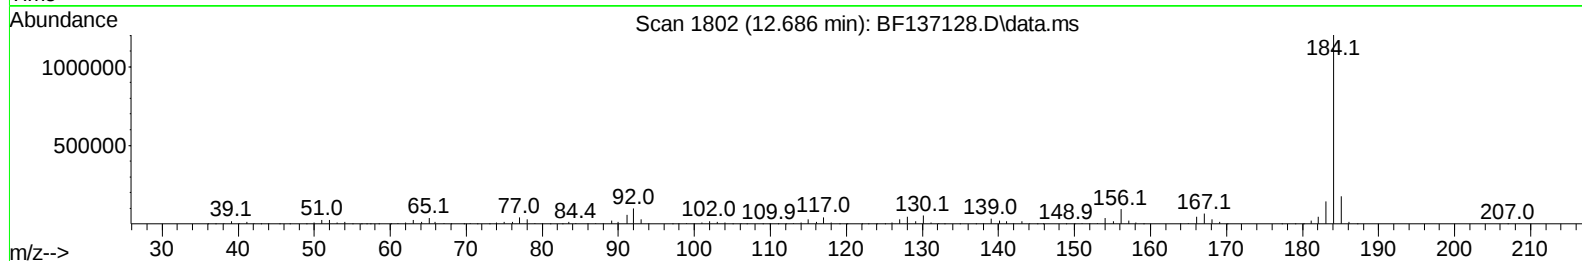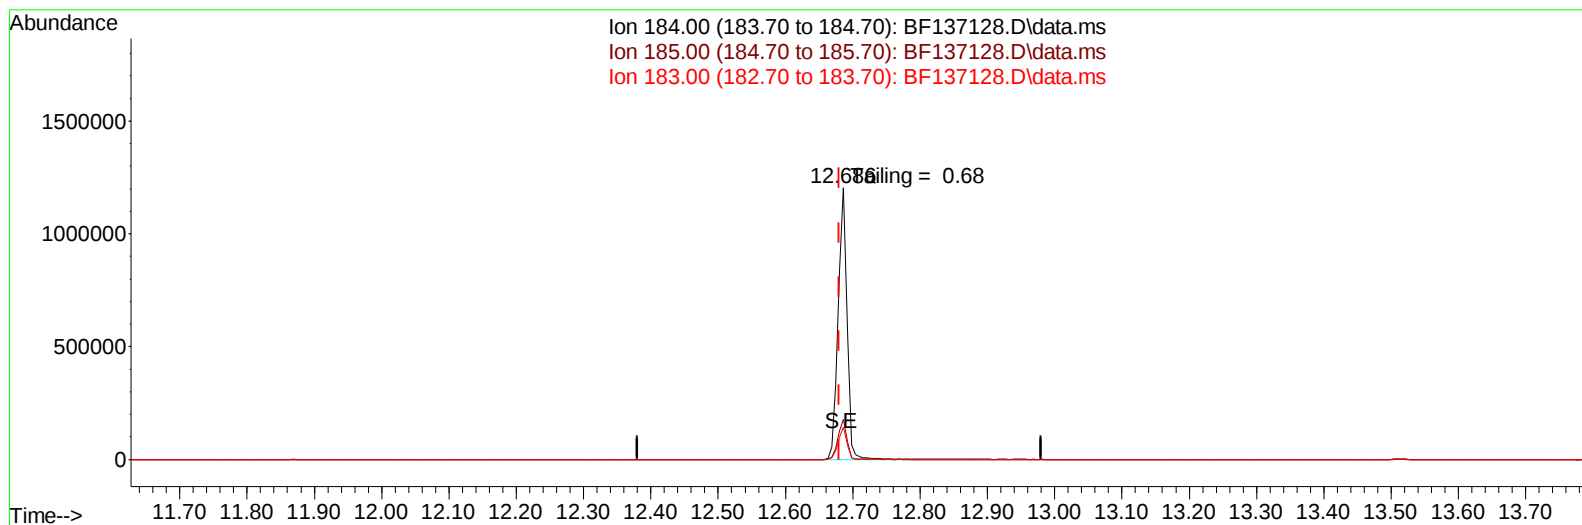

TIC: BF137128.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response 1092488

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.67
183.00	12.30	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/23/2024	BNA_F	<u>BF137128.D</u>
Compound Name	Response	Retention Time
DDT	314524	13.521
DDD	3903	13.216
DDE	0	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3903	318427	1.23

Instrument :
BNA_F
ClientSampleId :
DFTPP