
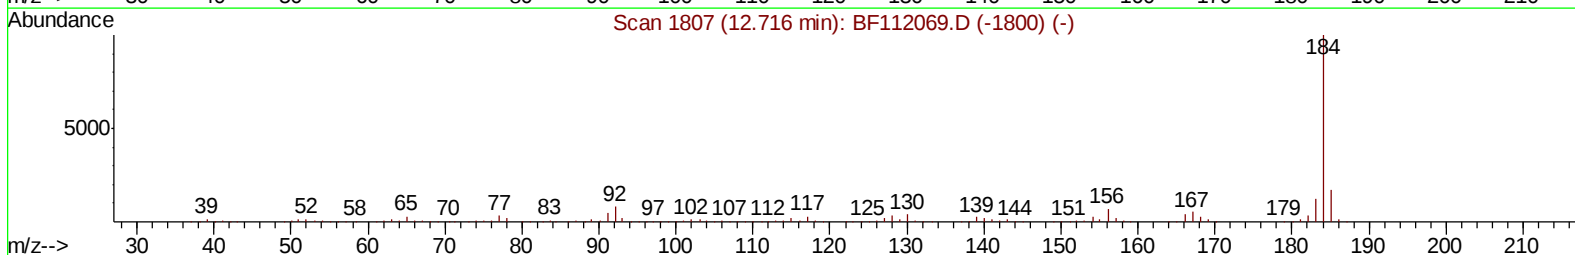
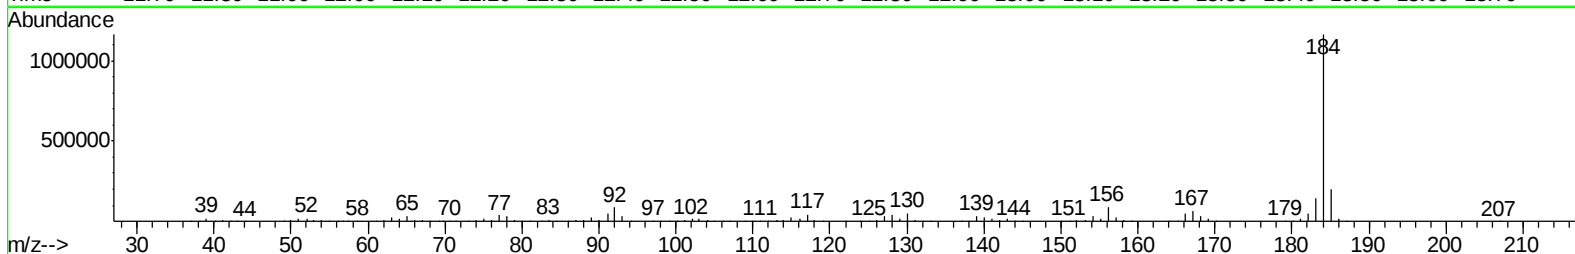


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012519\
 Data File : BF112237.D
 Acq On : 25 Jan 2019 17:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 01:33:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 00:11:07 2019
 Response via : Initial Calibration

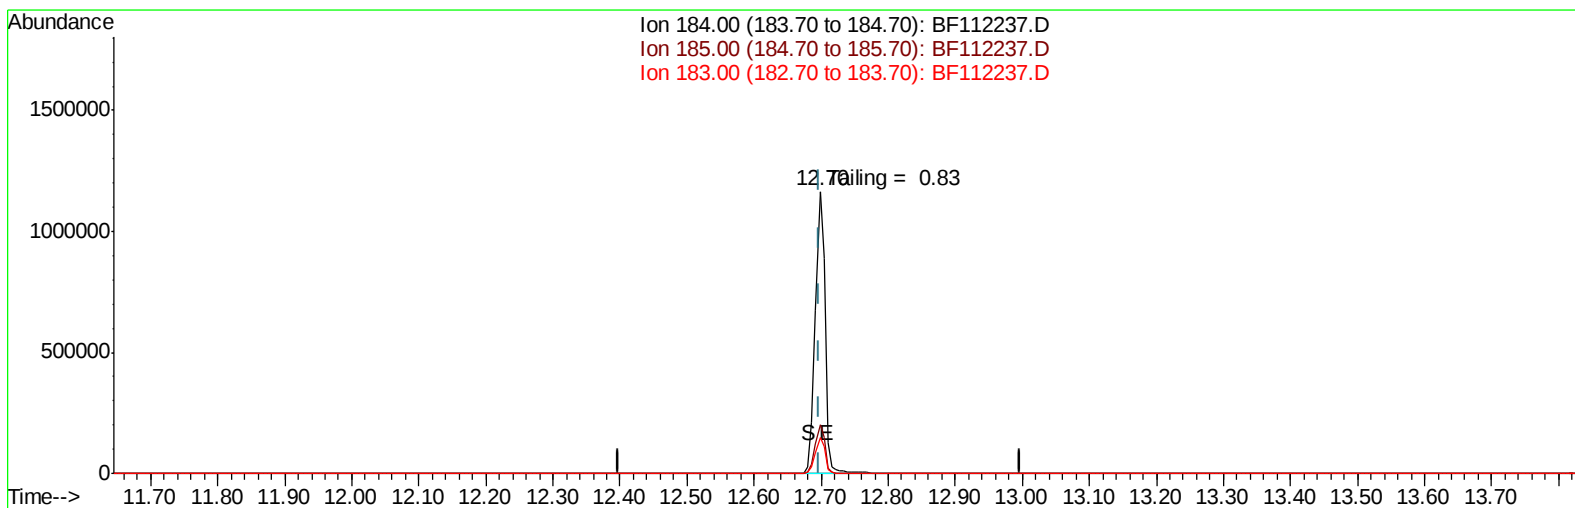

TIC: BF112237.D

(77) Benzidine




12.698min (0.000) 0.00ng

response 1127586

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	17.38
183.00	12.50	12.58
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012519\
Data File : BF112237.D
Acq On : 25 Jan 2019 17:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 01:33:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 00:11:07 2019
Response via : Initial Calibration

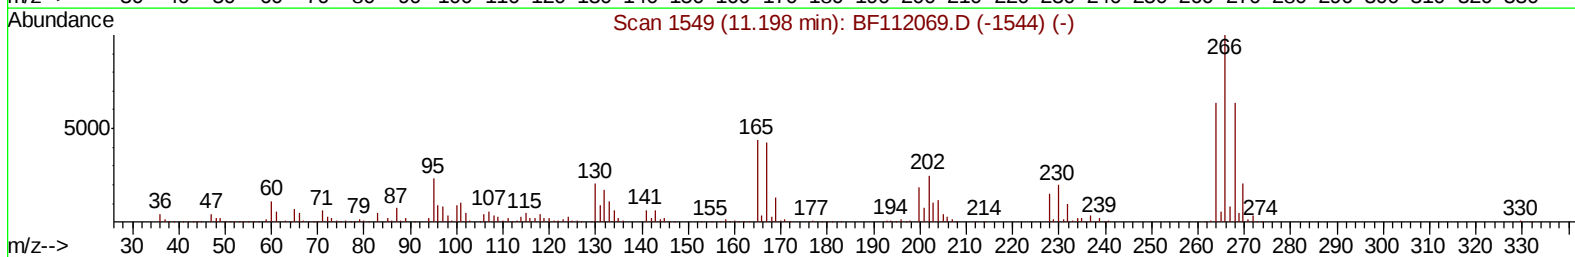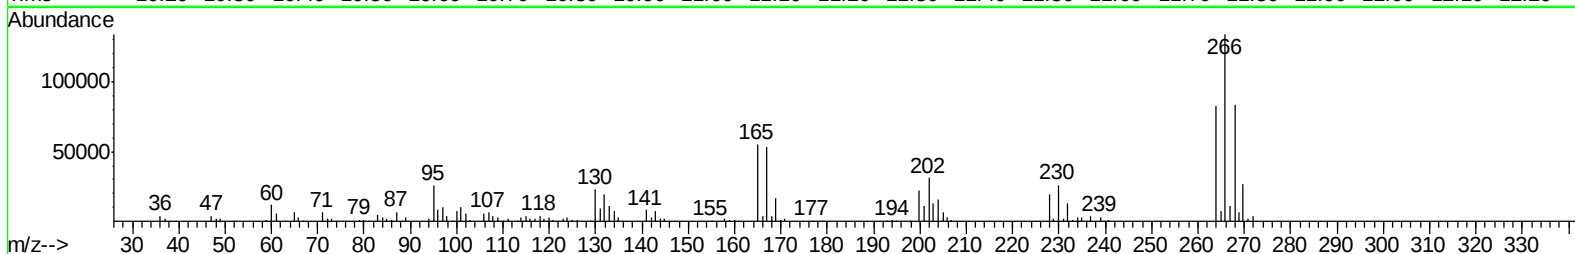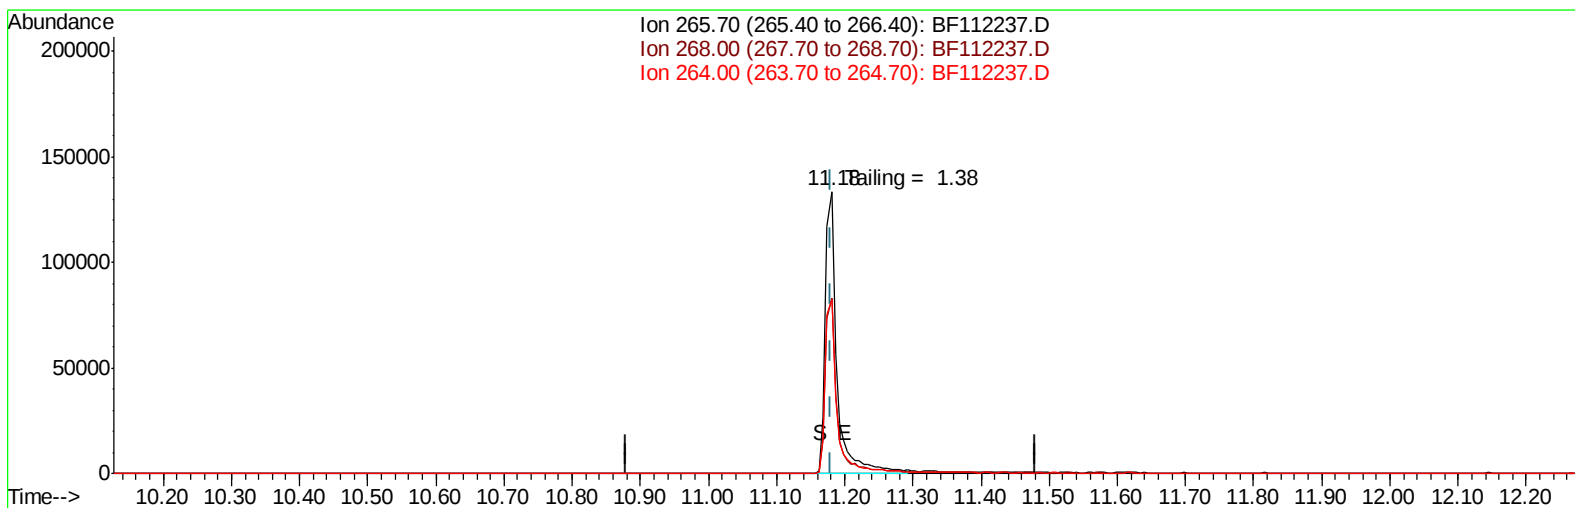

TIC: BF112237.D

(70) Pentachlorophenol (C)

11.180min (0.000) 276901.75ng

response 152273

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.36
264.00	63.60	61.76
0.00	0.00	0.00