

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012519\
 Data File : BF112248.D
 Acq On : 25 Jan 2019 22:45
 Operator : JU/SJ
 Sample : K1003-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-02-012319

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.381	43	50	51	rBV	1886110	4347727	69.80%	8.479%
2	2.881	130	135	146	rVB	249723	351956	5.65%	0.686%
3	4.663	433	438	445	rBV	160085	183002	2.94%	0.357%
4	5.081	505	509	519	rBV2	404125	722589	11.60%	1.409%
5	5.493	574	579	589	rBV	4376218	4197025	67.38%	8.185%
6	6.492	744	749	766	rBV	3843282	4015347	64.46%	7.831%
7	6.622	766	771	774	rBV	5433346	4948624	79.45%	9.651%
8	6.839	805	808	814	rBV	1277638	1086176	17.44%	2.118%
9	6.998	831	835	839	rBV	4445564	3988927	64.04%	7.780%
10	7.404	898	904	907	rBV	3243349	3145956	50.51%	6.136%
11	8.122	1021	1026	1040	rBV	1590223	1428249	22.93%	2.786%
12	9.198	1203	1209	1212	rBV	6454254	6228827	100.00%	12.148%
13	9.875	1318	1324	1334	rBV	1718387	1636384	26.27%	3.191%
14	10.669	1454	1459	1473	rBV	3754637	3659638	58.75%	7.137%
15	11.363	1573	1577	1585	rBV	1734095	1509083	24.23%	2.943%
16	12.827	1818	1826	1841	rBV	1139533	1655966	26.59%	3.230%
17	12.945	1841	1846	1849	rBV	5346484	4950444	79.48%	9.655%
18	13.145	1877	1880	1890	rBV	306162	302802	4.86%	0.591%
19	13.998	2022	2025	2032	rVB	1071451	983083	15.78%	1.917%
20	14.457	2098	2103	2110	rBV	95209	113072	1.82%	0.221%
21	14.757	2149	2154	2158	rBV	128948	145574	2.34%	0.284%
22	15.092	2207	2211	2220	rVB	139404	167043	2.68%	0.326%
23	15.462	2269	2274	2286	rVB	890786	1176559	18.89%	2.295%
24	15.898	2342	2348	2353	rBV2	123250	191569	3.08%	0.374%
25	16.398	2428	2433	2439	rBV	87875	138667	2.23%	0.270%


Sum of corrected areas: 51274289

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012519\
Data File : BF112248.D
Acq On : 25 Jan 2019 22:45
Operator : JU/SJ
Sample : K1003-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
BU-02-012319

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

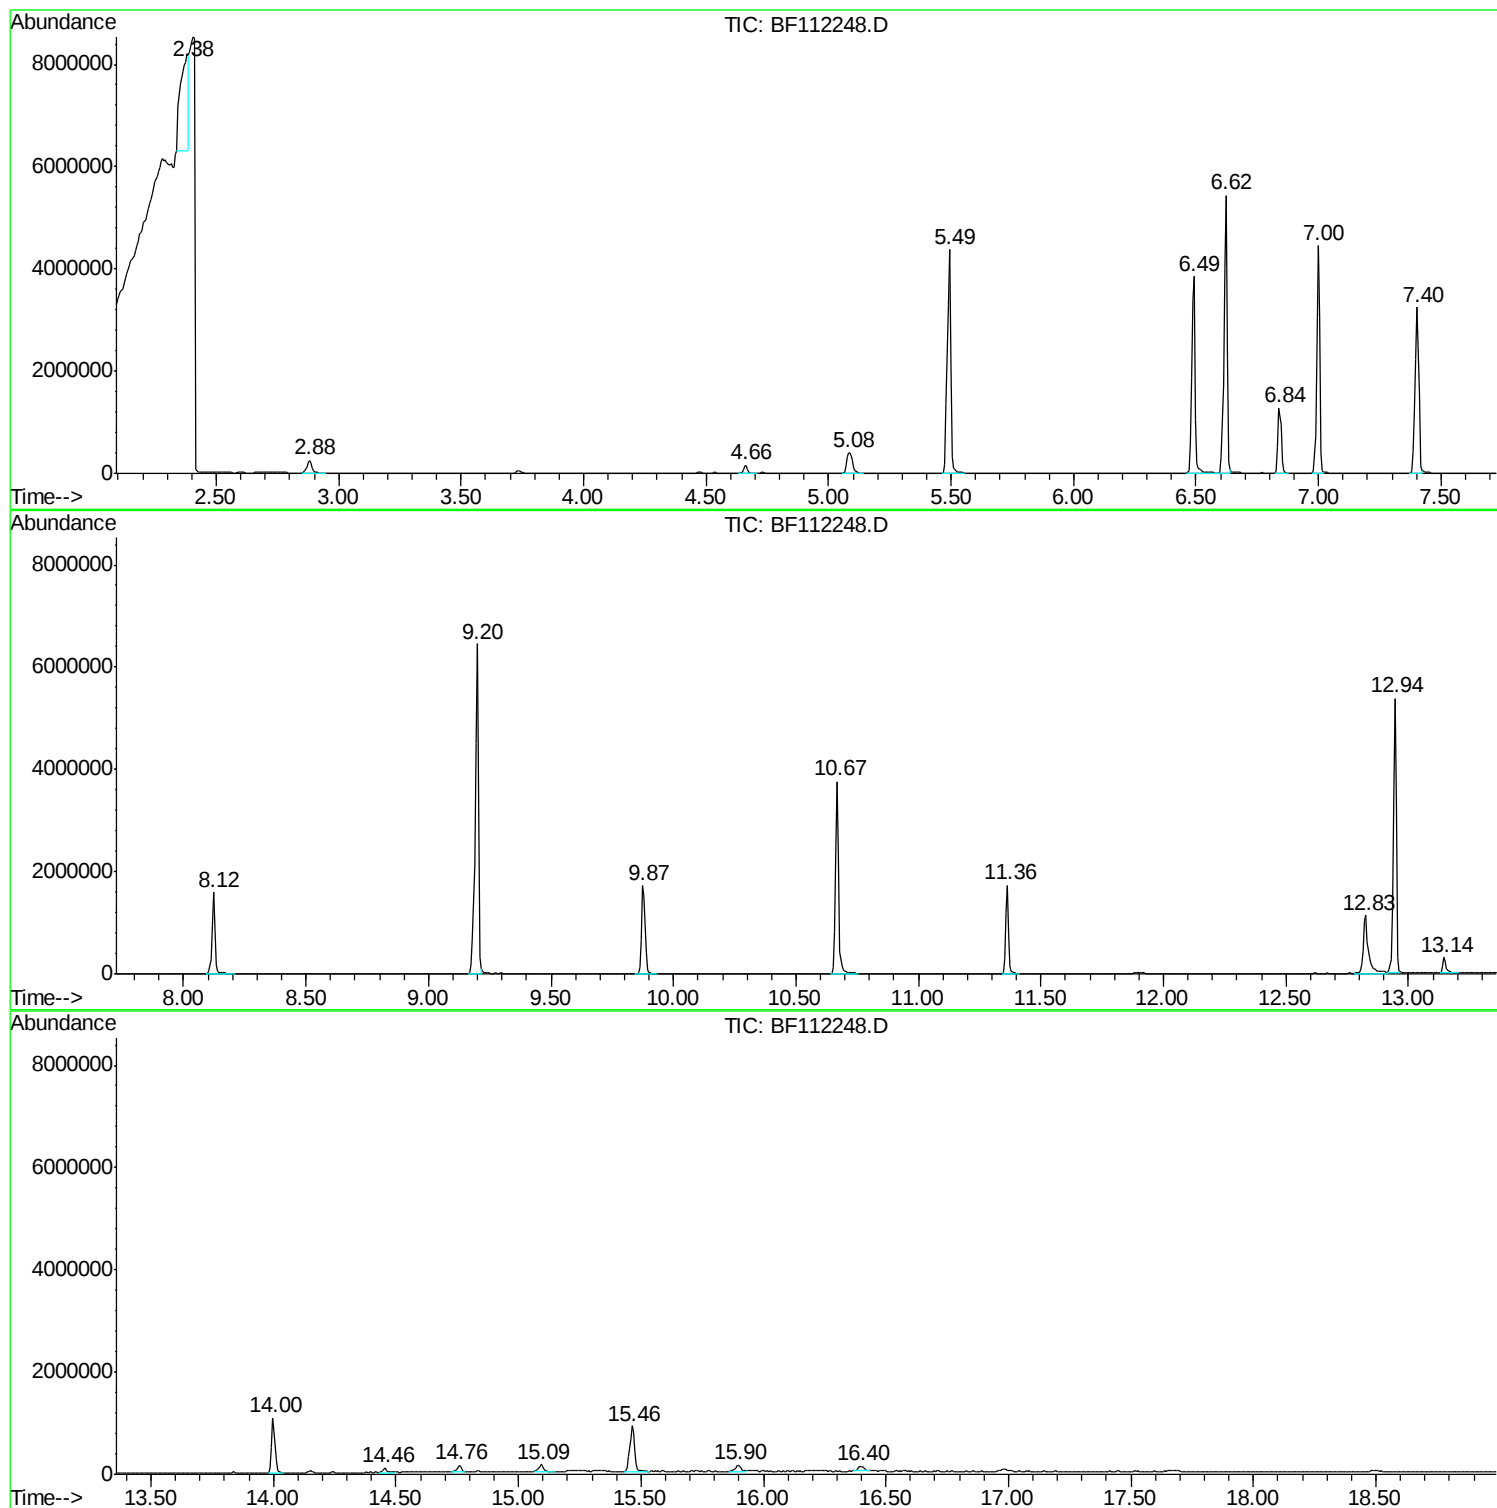

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012519\
Data_File : BF112248.D
Acq_On : 25-Jan-2019 22:455
Operator : JU/SJJ
Sample : K1003-022
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
BU-02-012319

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
