


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF012519\  
 Data File : BF112226.D  
 Acq On : 25 Jan 2019 11:03  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012519.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jan 28 02:58:56 2019

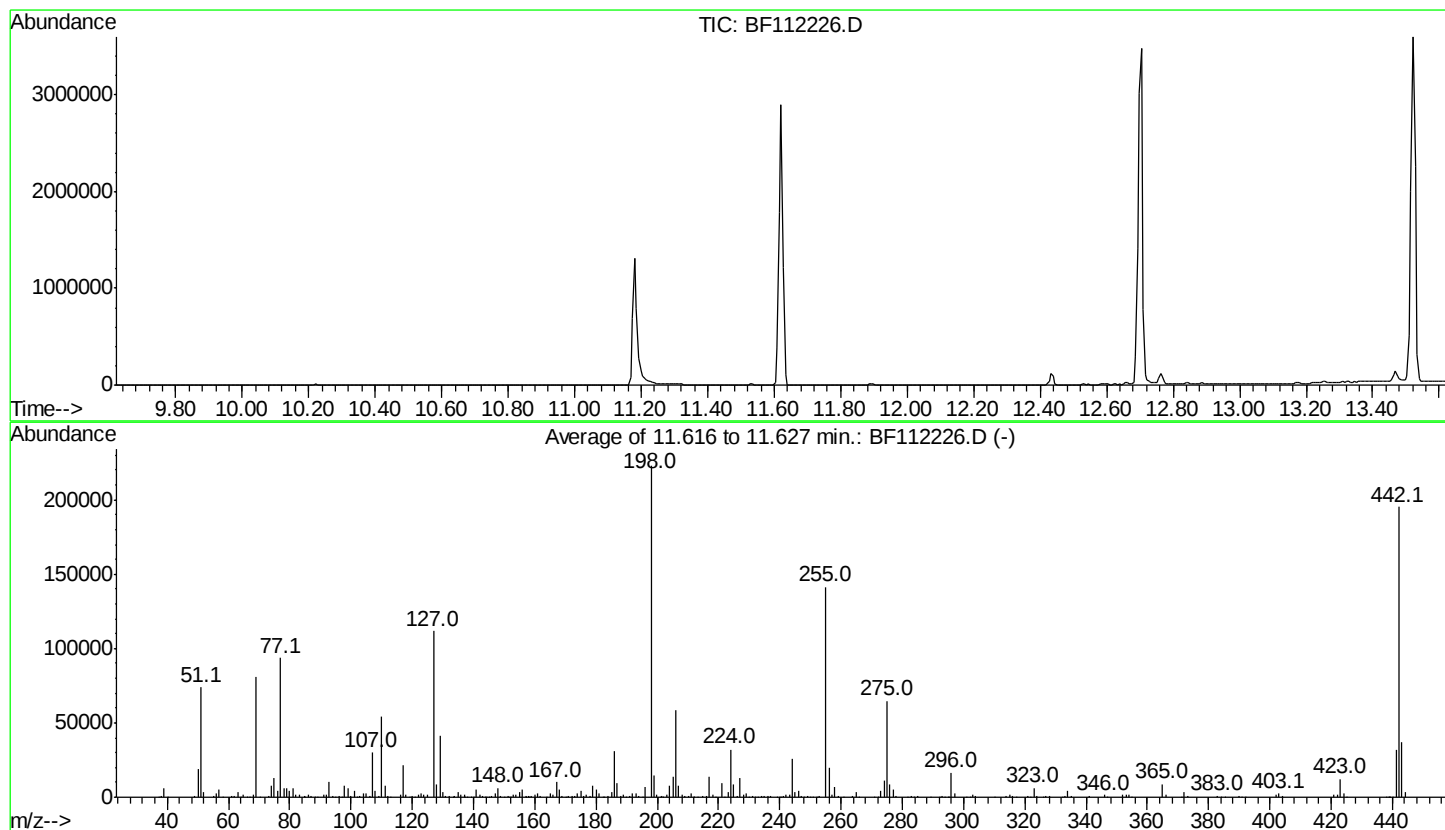

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 33.1         | 73741      | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 1609       | PASS                |
| 69             | 198             | 0.00            | 100             | 36.2         | 80810      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 400        | PASS                |
| 127            | 198             | 10              | 80              | 50.1         | 111824     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 222994     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 14947      | PASS                |
| 275            | 198             | 10              | 60              | 29.1         | 65002      | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 8862       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.2         | 31655      | PASS                |
| 442            | 198             | 50              | 100             | 87.5         | 195085     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 36762      | PASS                |