


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012519\
 Data File : BF112237.D
 Acq On : 25 Jan 2019 17:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 02:58:56 2019

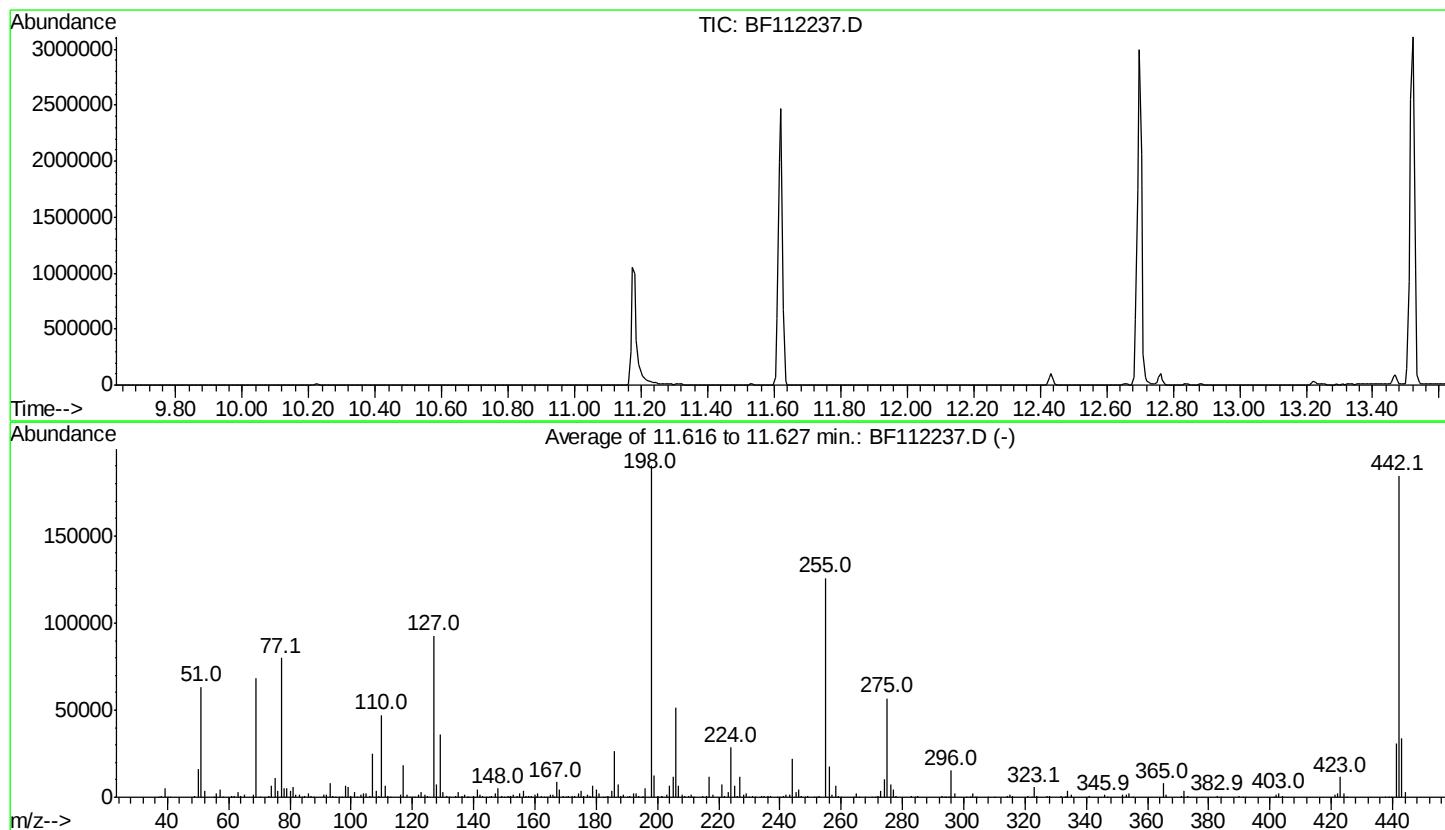

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	63390	PASS
68	69	0.00	2	2.0	1356	PASS
69	198	0.00	100	35.9	68325	PASS
70	69	0.00	2	0.5	325	PASS
127	198	10	80	48.8	92885	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	190301	PASS
199	198	5	9	6.8	12851	PASS
275	198	10	60	29.8	56709	PASS
365	198	1	100	4.1	7781	PASS
441	198	0.01	100	16.1	30592	PASS
442	198	50	100	97.1	184754	PASS
443	442	15	24	18.3	33877	PASS