
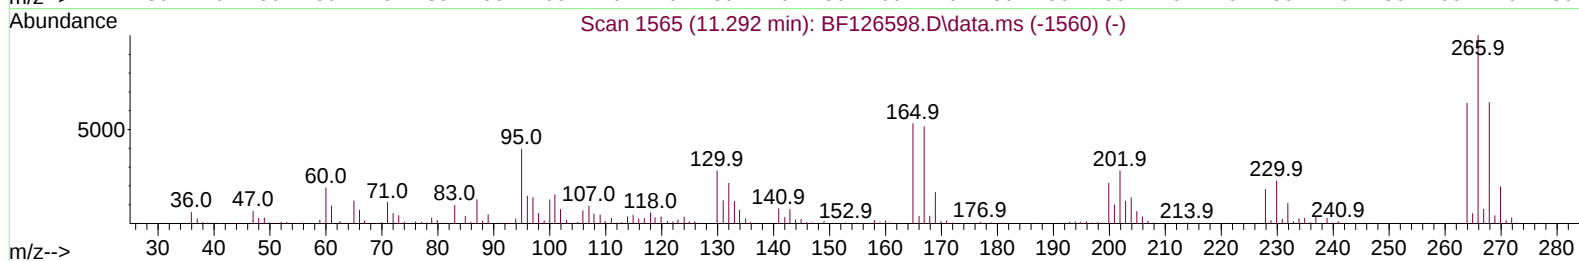
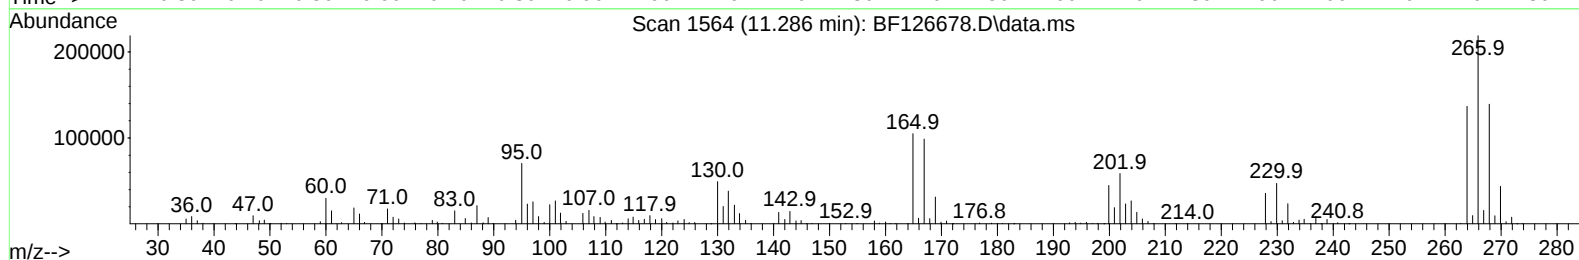


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012622\
 Data File : BF126678.D
 Acq On : 26 Jan 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 08:23:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 27 03:09:40 2022
 Response via : Initial Calibration

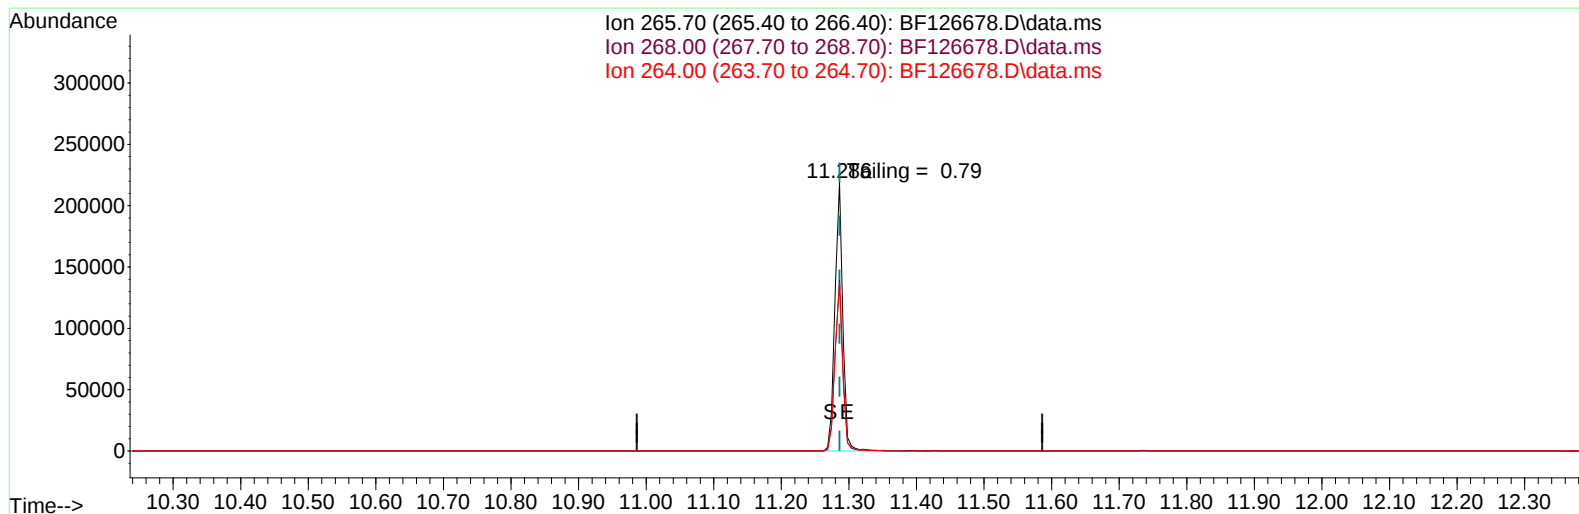

TIC: BF126678.D\data.ms

(70) Pentachlorophenol (C)




11.286min (-0.000) 31621.65 ng

response 176814

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	63.67
264.00	63.00	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012622\
Data File : BF126678.D
Acq On : 26 Jan 2022 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 08:23:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration

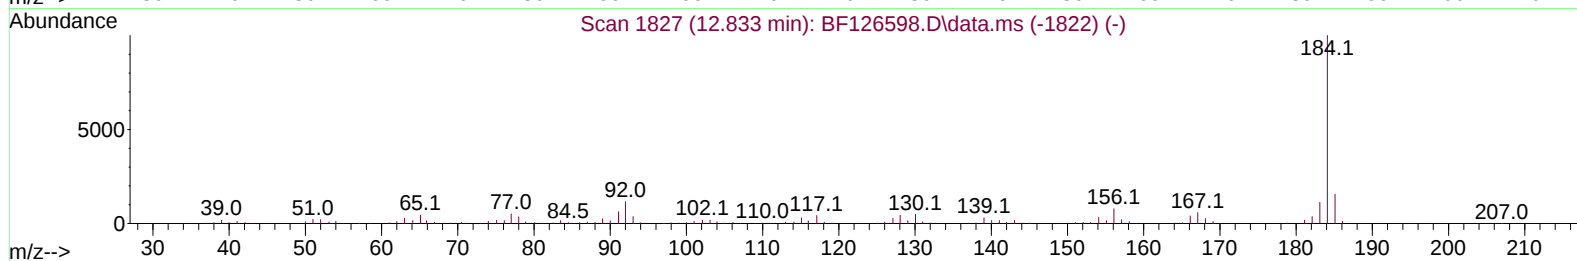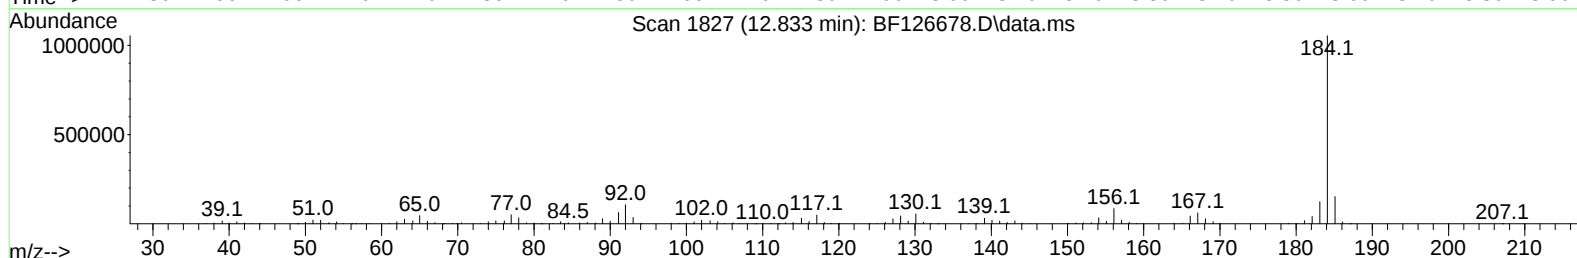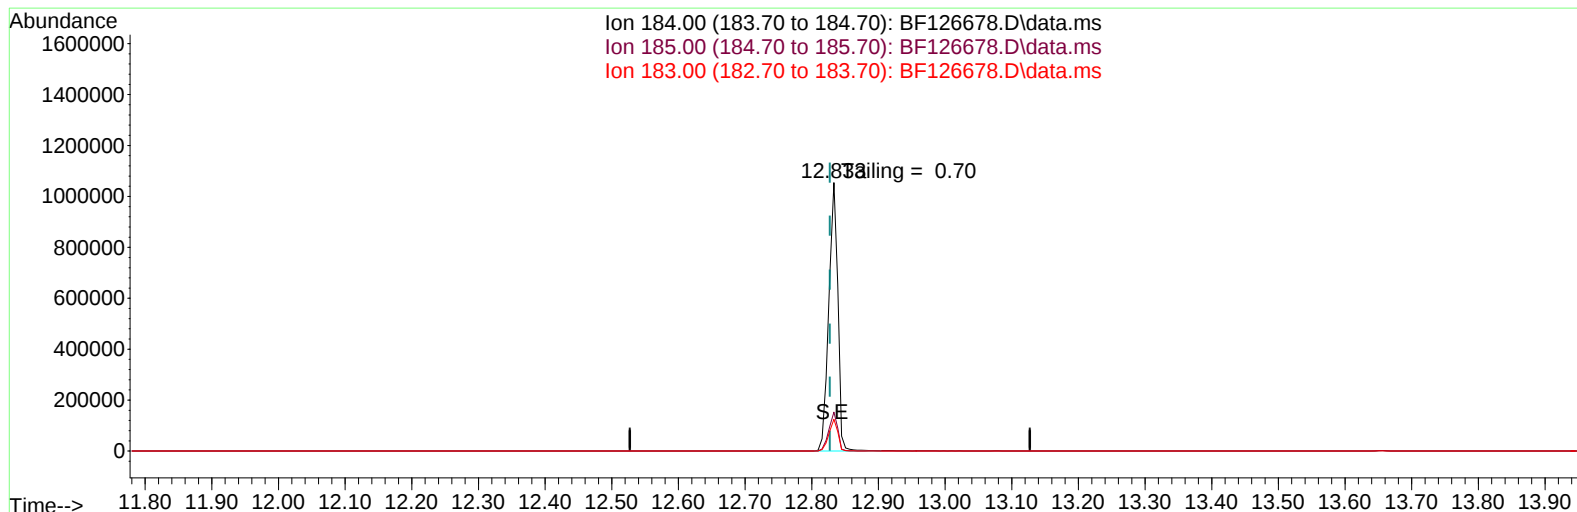

TIC: BF126678.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 0.00 ng

response 1005689

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.52
183.00	10.20	11.80
0.00	0.00	0.00