
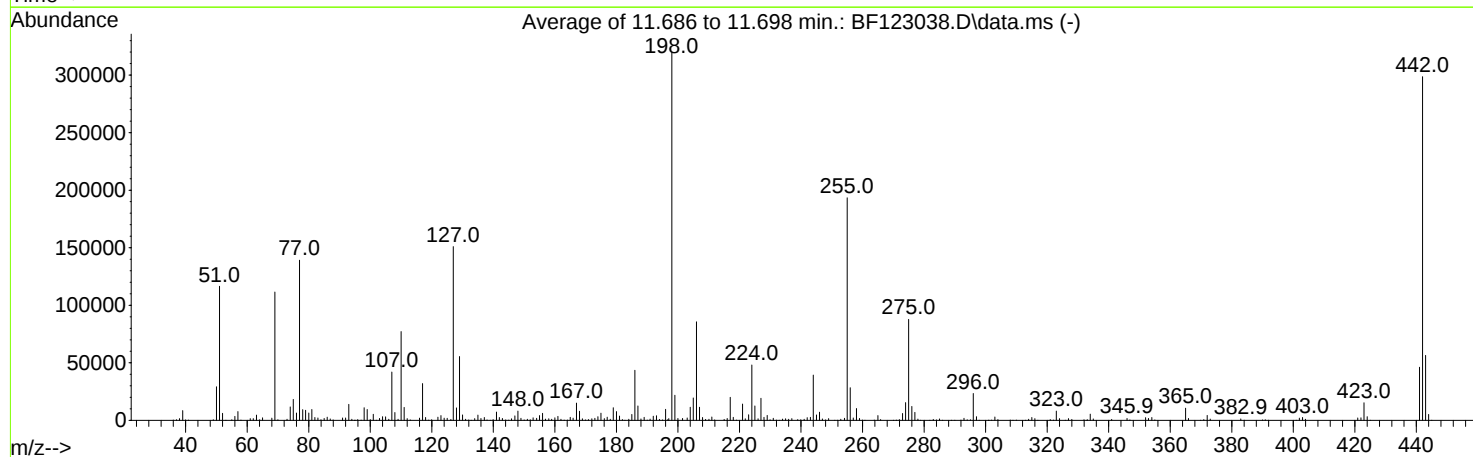


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012721\
 Data File : BF123038.D
 Acq On : 27 Jan 2021 11:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 28 00:48:07 2021

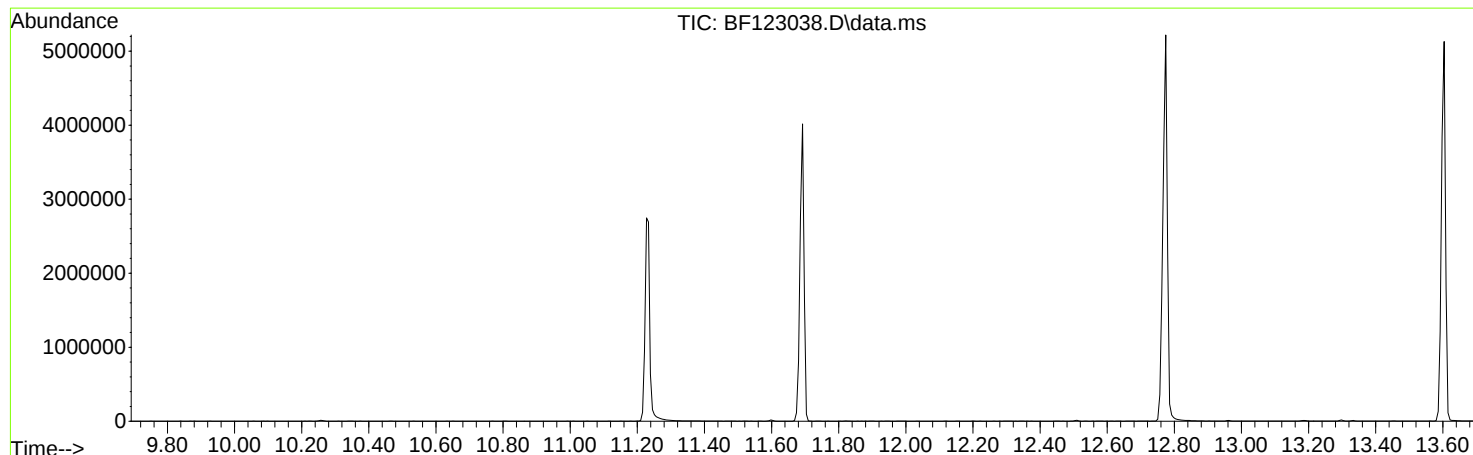

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	116453	PASS
68	69	0.00	2	1.7	1925	PASS
69	198	0.00	100	34.9	111475	PASS
70	69	0.00	2	0.5	518	PASS
127	198	10	80	47.2	150987	PASS
197	198	0.00	2	0.5	1589	PASS
198	198	100	100	100.0	319659	PASS
199	198	5	9	6.8	21848	PASS
275	198	10	60	27.5	87779	PASS
365	198	1	100	3.3	10608	PASS
441	198	0.01	100	14.4	46171	PASS
442	442	50	100	100.0	298645	PASS
443	442	15	24	18.9	56483	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2021	BNA_F	<u>BF123038.D</u>
Compound Name	Response	Retention Time
DDT	842651	13.604
DDD	5893	13.298
DDE	1708	12.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7601	850252	0.89

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012721\
 Data File : BF123038.D
 Acq On : 27 Jan 2021 11:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 06:44:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 28 00:48:07 2021
 Response via : Initial Calibration

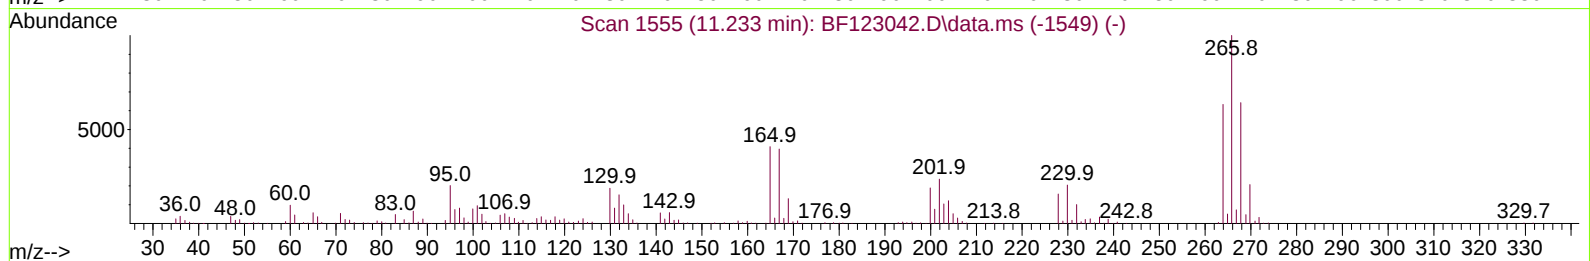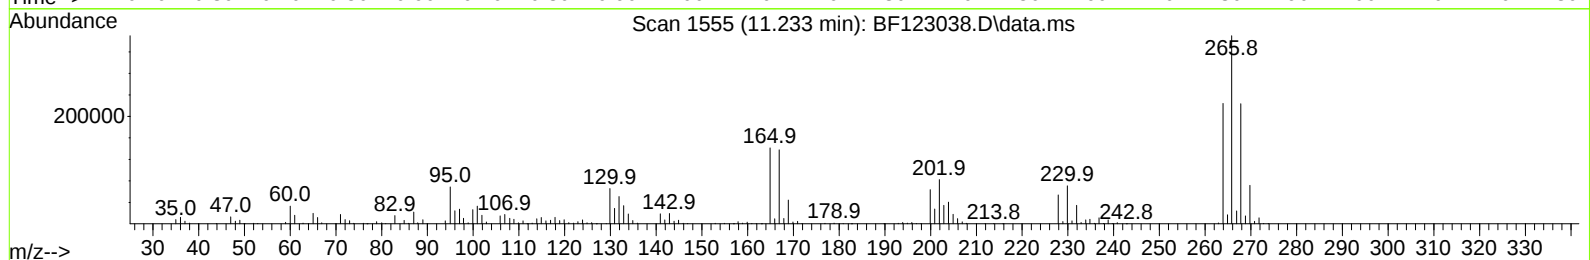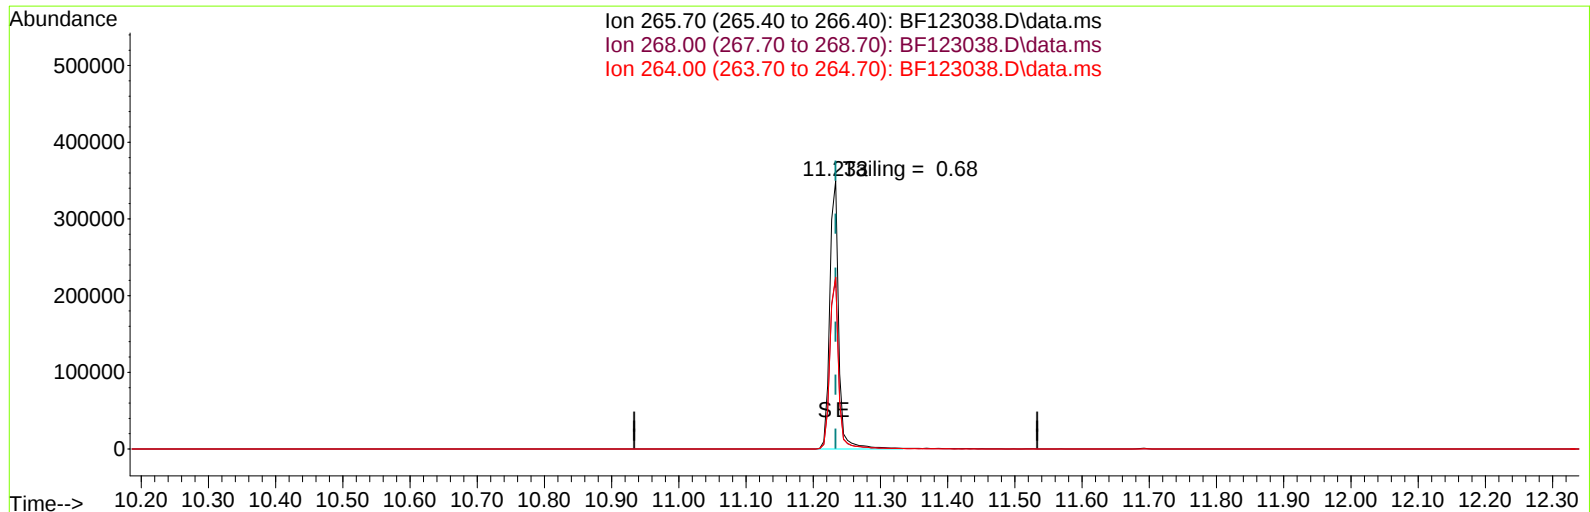

TIC: BF123038.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 29968.74 ng




response 322589

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.86
264.00	62.30	64.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012721\
Data File : BF123038.D
Acq On : 27 Jan 2021 11:29
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 28 06:44:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 28 00:48:07 2021
Response via : Initial Calibration

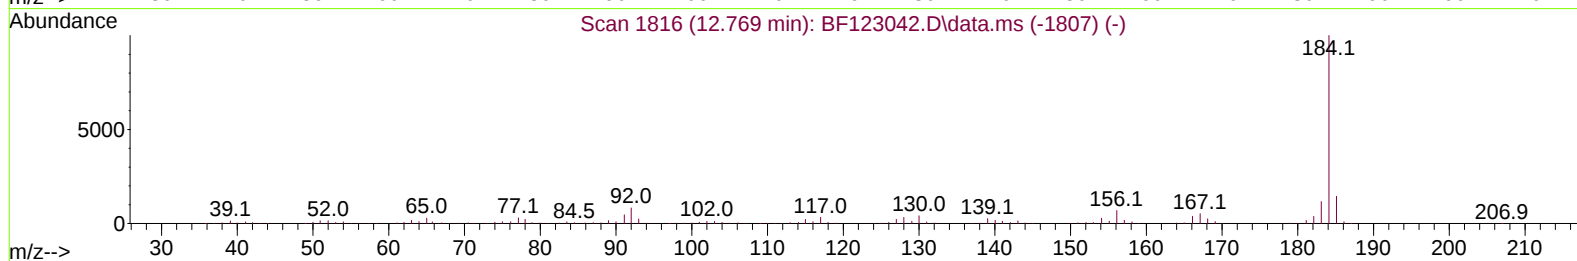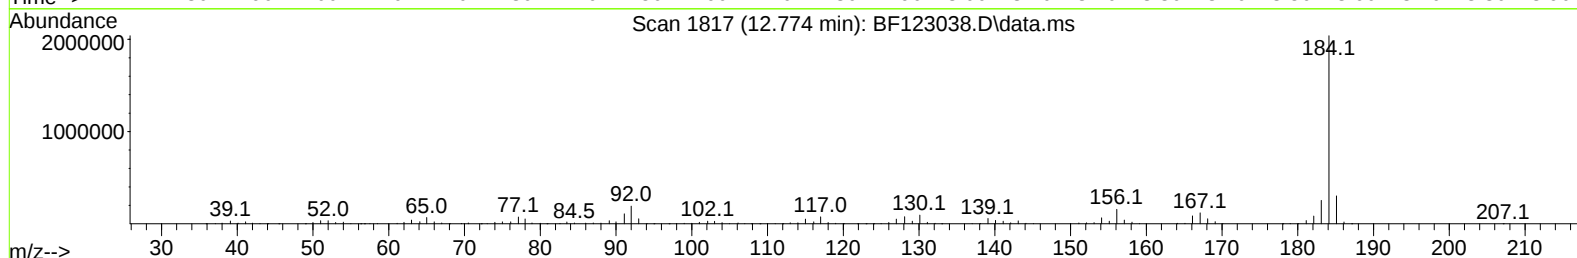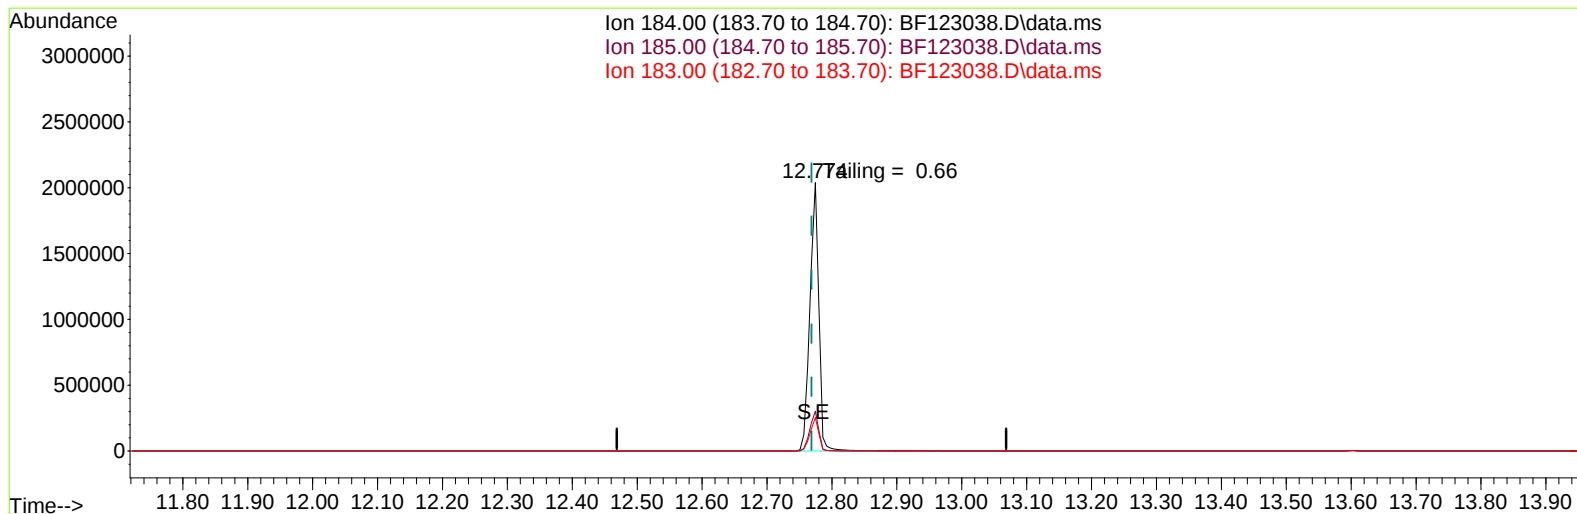

TIC: BF123038.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 1952386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.84
183.00	12.10	12.46
0.00	0.00	0.00