
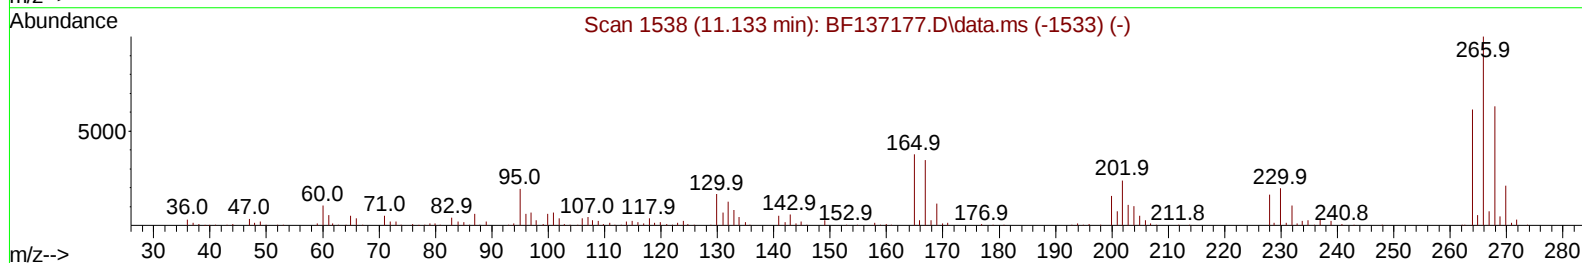
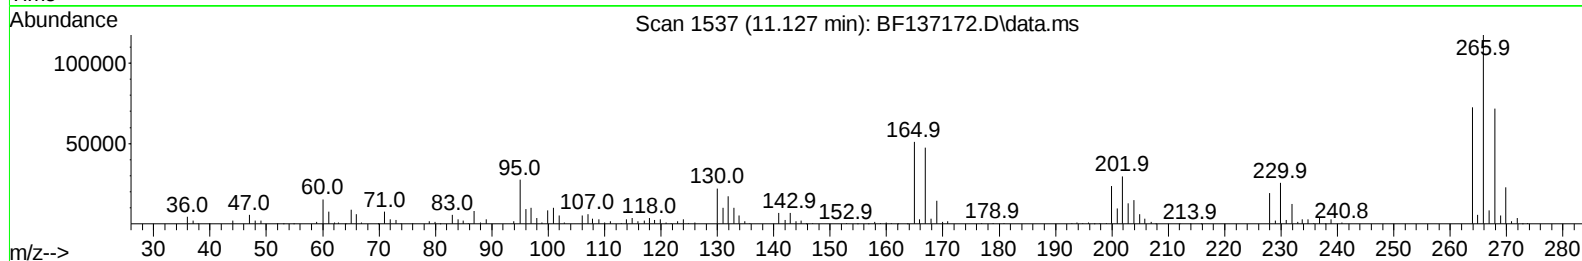


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012724\
Data File : BF137172.D
Acq On : 26 Jan 2024 18:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 02:20:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

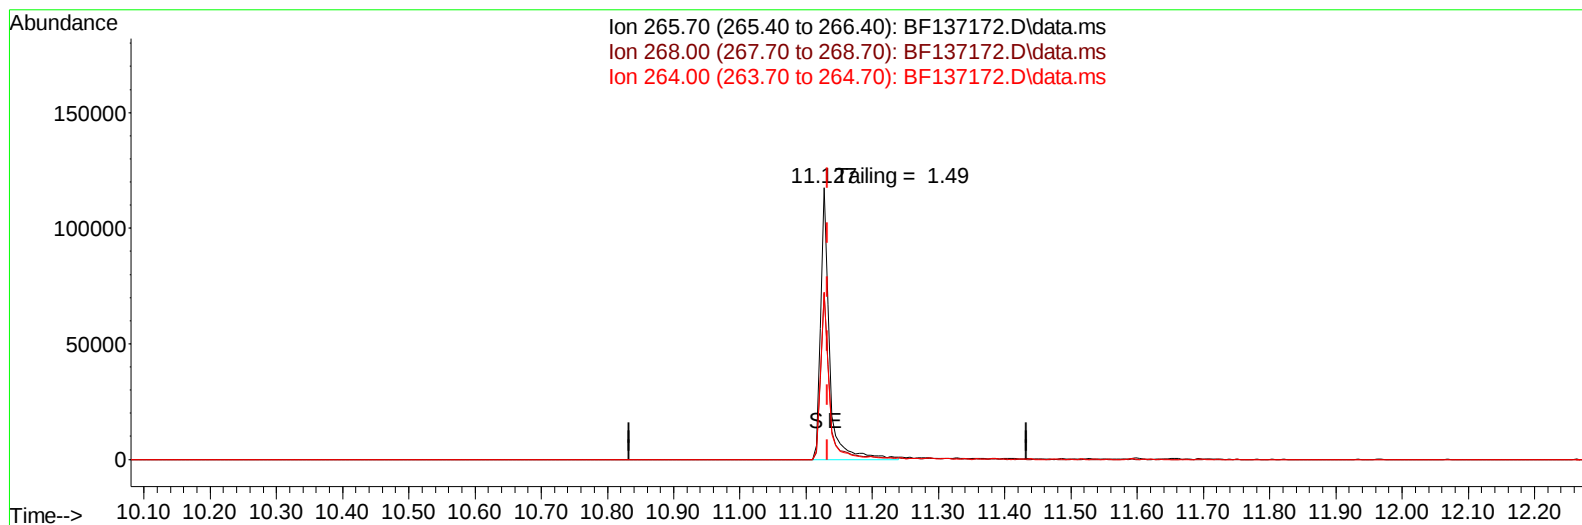




TIC: BF137172.D\data.ms

(70) Pentachlorophenol (C)**11.127min (-0.006) 34295.07 ng****response 112717**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.24
264.00	61.40	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012724\
Data File : BF137172.D
Acq On : 26 Jan 2024 18:14
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 02:20:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

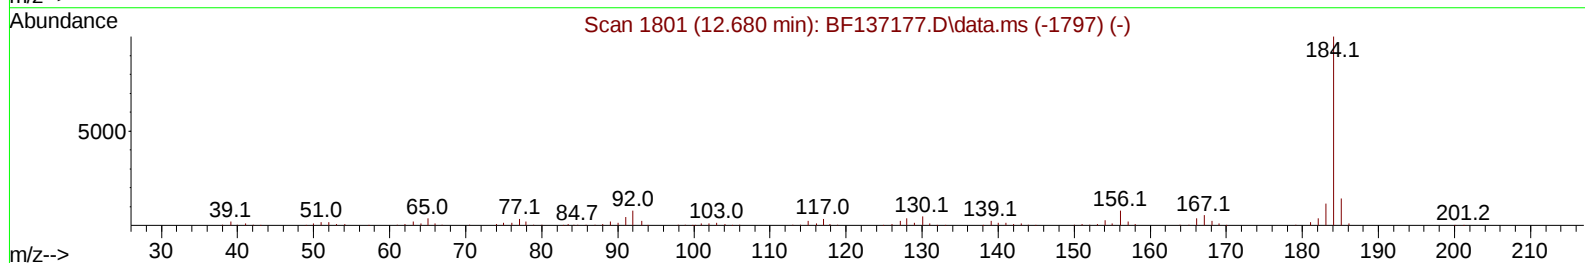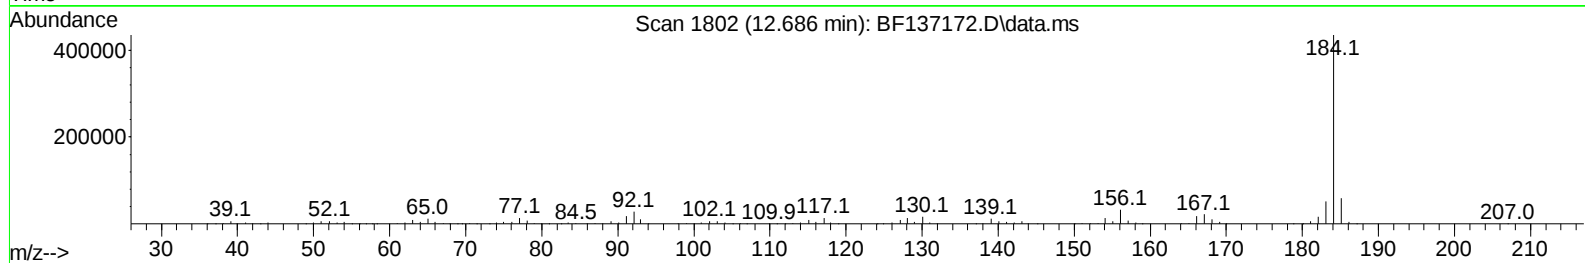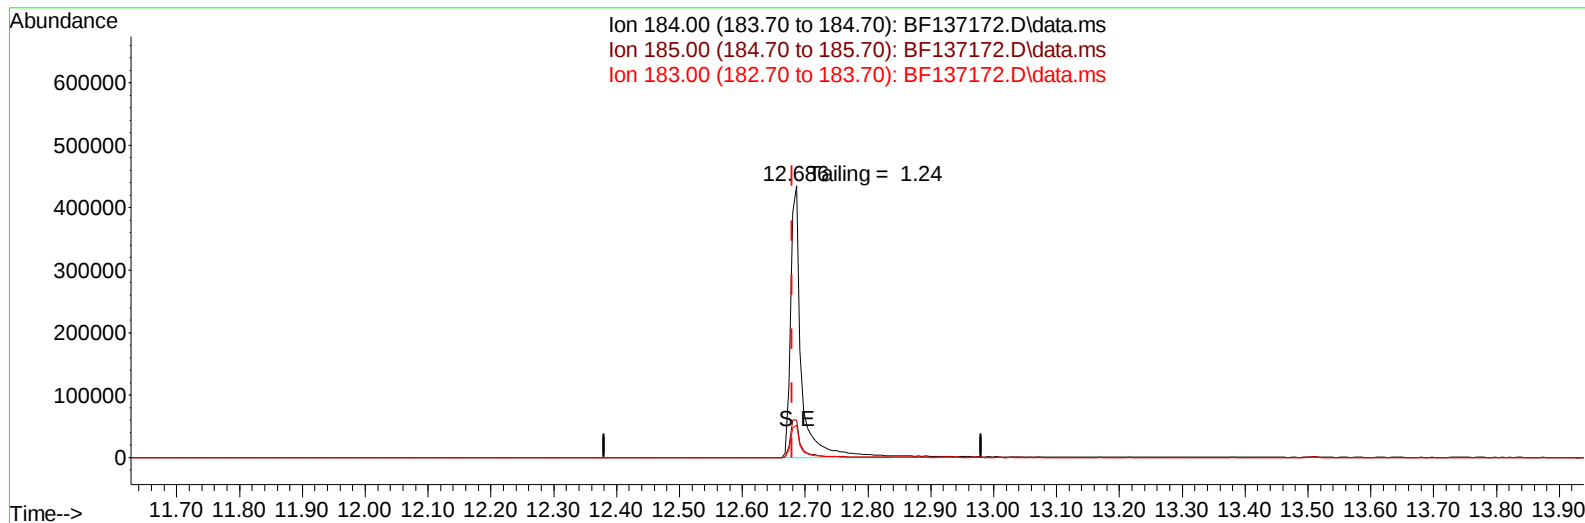

TIC: BF137172.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response 531470

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.76
183.00	11.50	11.89
0.00	0.00	0.00