


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012724\
Data File : BF137172.D
Acq On : 26 Jan 2024 18:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 27 02:14:33 2024

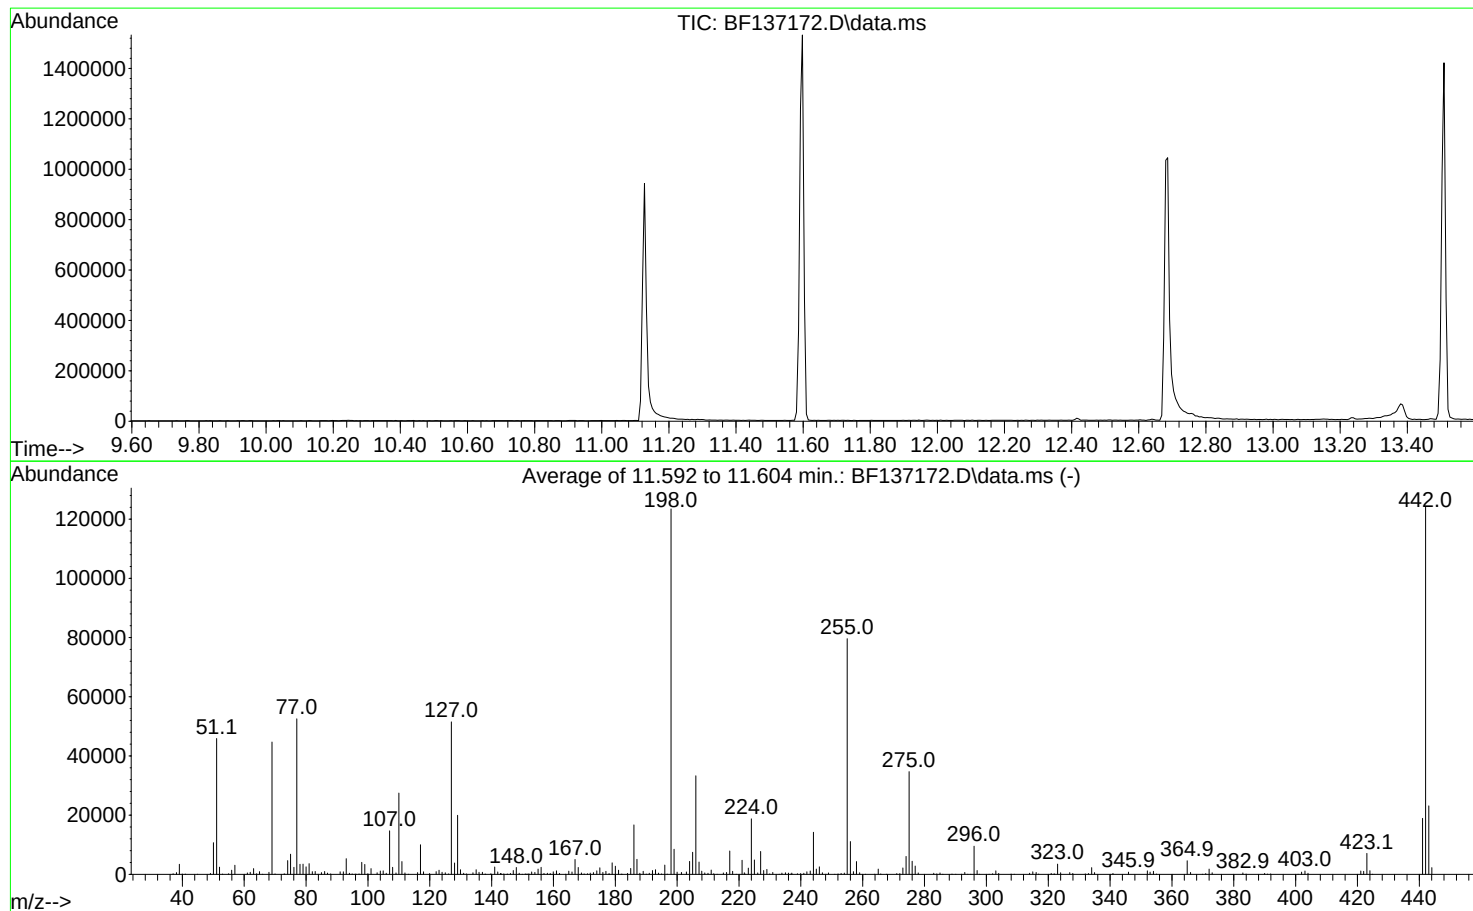




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	45869	PASS
68	69	0.00	2	1.5	682	PASS
69	198	0.00	100	36.2	44703	PASS
70	69	0.00	2	0.4	179	PASS
127	198	10	80	41.7	51489	PASS
197	198	0.00	2	0.1	126	PASS
198	198	100	100	100.0	123443	PASS
199	198	5	9	6.9	8503	PASS
275	198	10	60	28.1	34715	PASS
365	198	1	100	3.7	4622	PASS
441	198	0.01	100	15.3	18934	PASS
442	442	50	100	100.0	124251	PASS
443	442	15	24	18.6	23136	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012724\
Data File : BF137172.D
Acq On : 26 Jan 2024 18:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 27 02:20:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

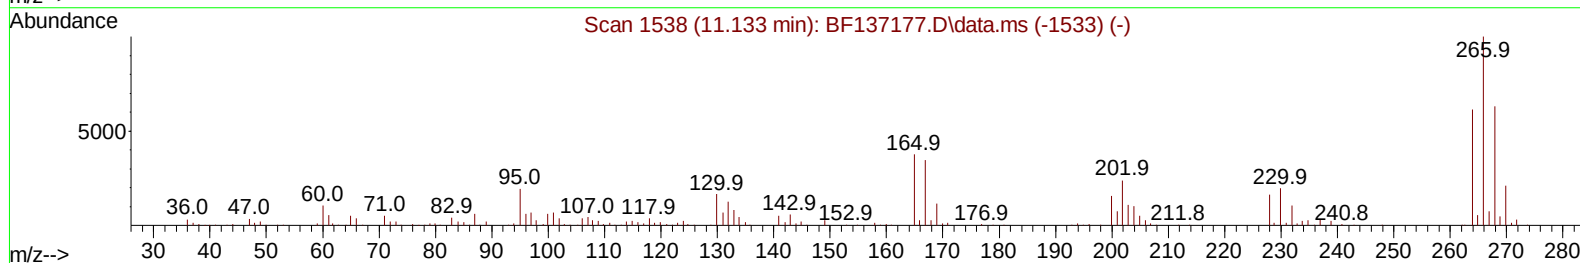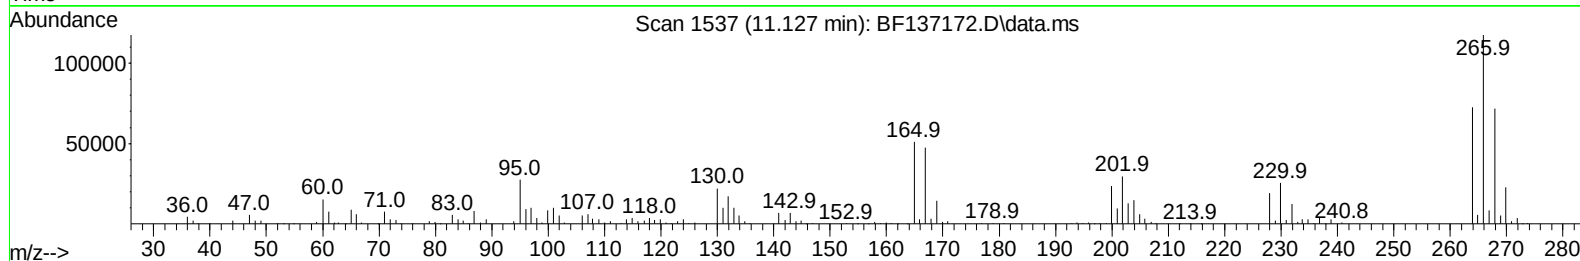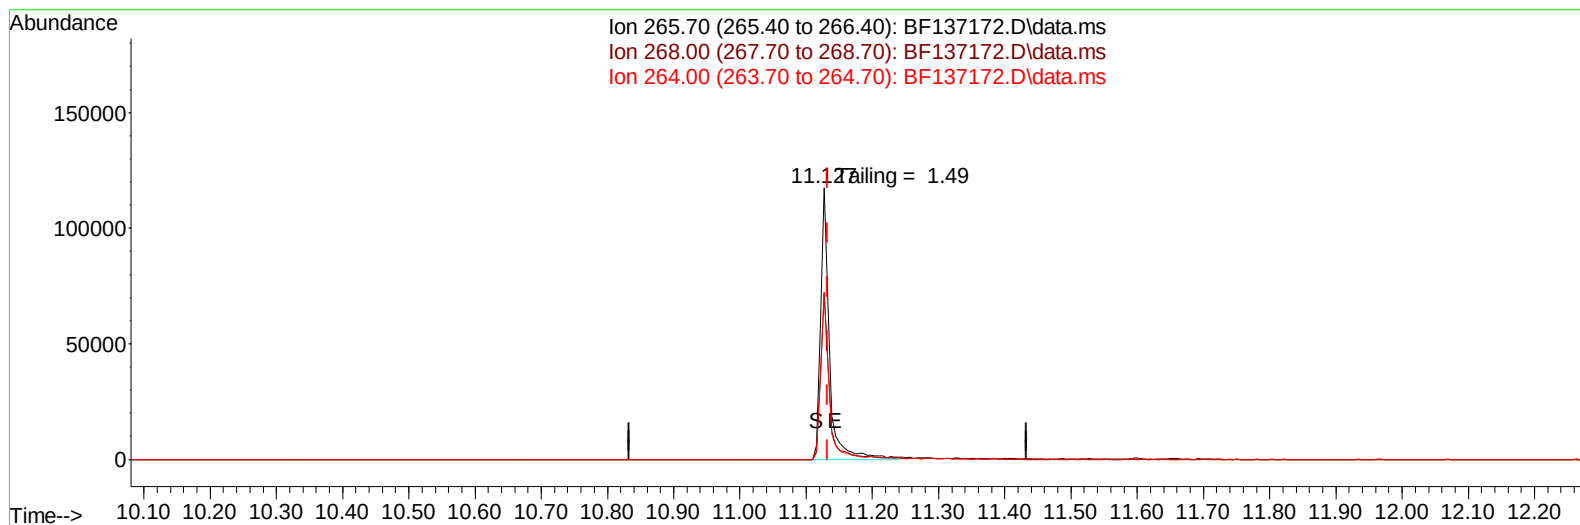

TIC: BF137172.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.006) 34295.07 ng




response 112717

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.24
264.00	61.40	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012724\
Data File : BF137172.D
Acq On : 26 Jan 2024 18:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 27 02:20:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

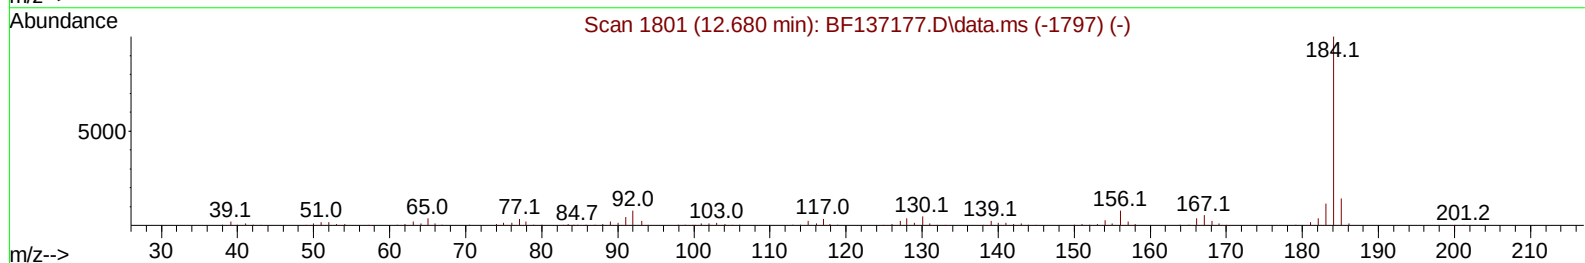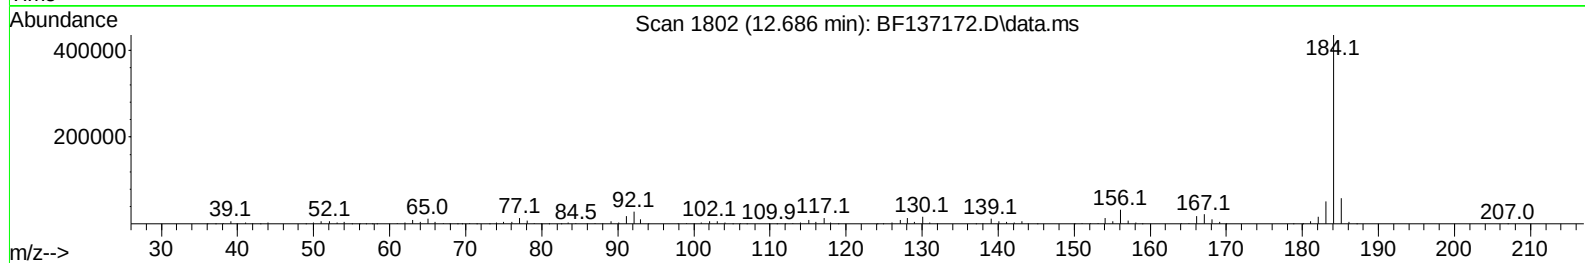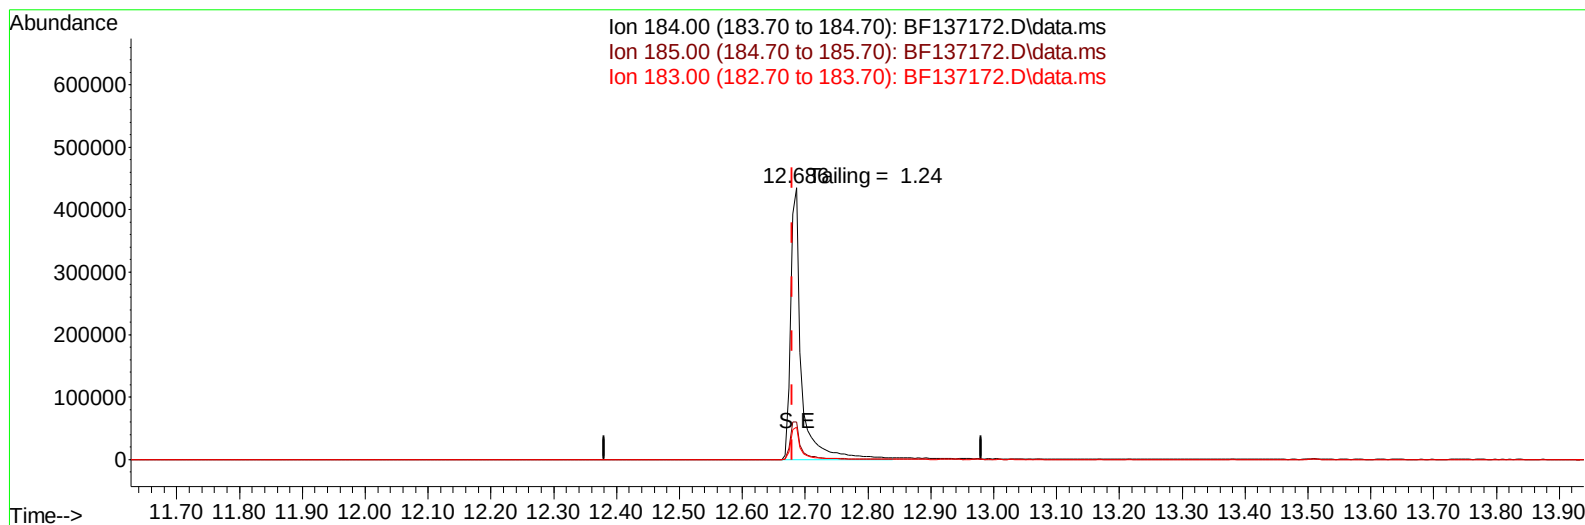

TIC: BF137172.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response 531470

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.76
183.00	11.50	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2024	BNA_F	<u>BF137172.D</u>
Compound Name	Response	Retention Time
DDT	209203	13.51
DDD	2227	13.21
DDE	0	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2227	211430	1.05

Instrument :
BNA_F
ClientSampleId :
DFTPP