

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012819\
 Data File : BM018665.D
 Acq On : 28 Jan 2019 15:43
 Operator : JU/SJ
 Sample : K1252-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GEN-1

Quant Time: Jan 28 16:21:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 22:01:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	206151	20.00	ng	-0.01
21) Naphthalene-d8	10.52	136	816095	20.00	ng	-0.01
39) Acenaphthene-d10	14.37	164	460181	20.00	ng	-0.01
64) Phenanthrene-d10	17.13	188	1034022	20.00	ng	-0.01
76) Chrysene-d12	21.32	240	1104454	20.00	ng	-0.01
87) Perylene-d12	23.59	264	1120911	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	1175459	105.29	ng	-0.01
7) Phenol-d6	6.90	99	1646222	116.09	ng	-0.01
23) Nitrobenzene-d5	8.89	82	1047154	74.38	ng	-0.01
42) 2,4,6-Tribromophenol	15.87	330	605305	103.31	ng	-0.02
45) 2-Fluorobiphenyl	12.99	172	2647336	75.07	ng	-0.01
79) Terphenyl-d14	19.76	244	3990782	76.17	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.84	163	149033	3.943	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012819\
Data File : BM018665.D
Acq On : 28 Jan 2019 15:43
Operator : JU/SJ
Sample : K1252-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GEN-1

Quant Time: Jan 28 16:21:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

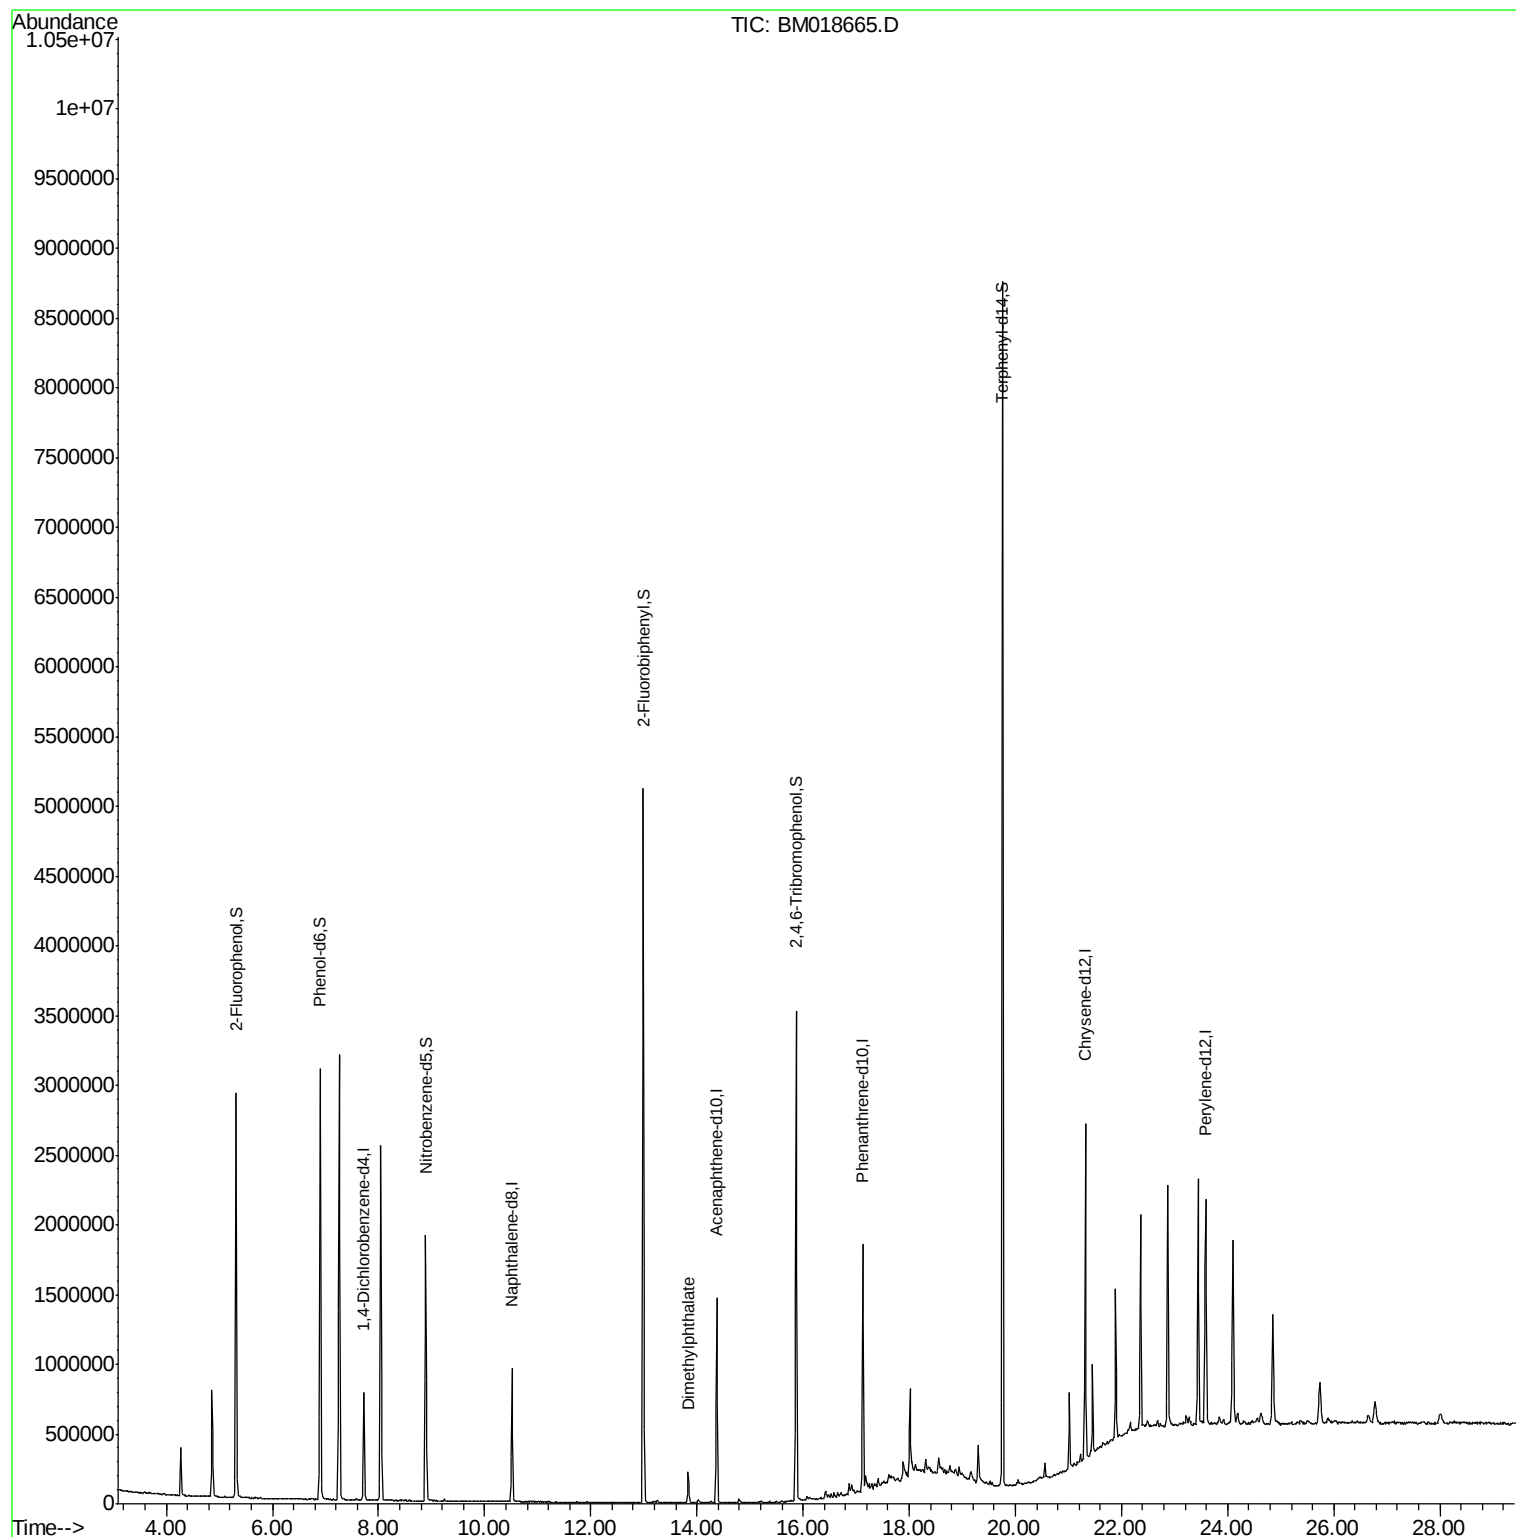

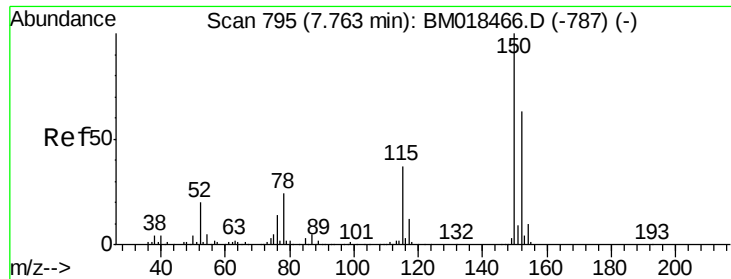


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BM018665.D
Acq: 28 Jan 2019 15:43

Instrument :
BNA_F
ClientSampleId :
GEN-1

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.0	126.9	190.3
115	56.6	45.5	68.3



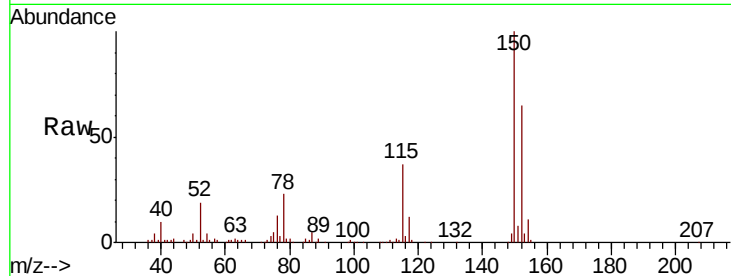


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

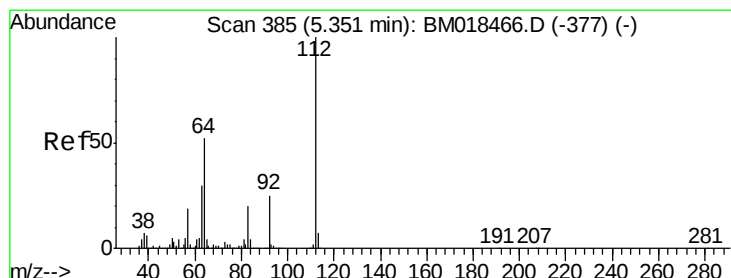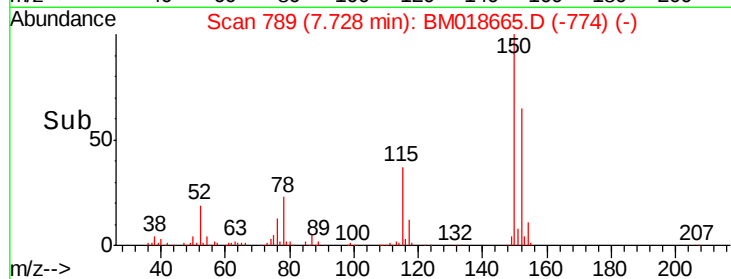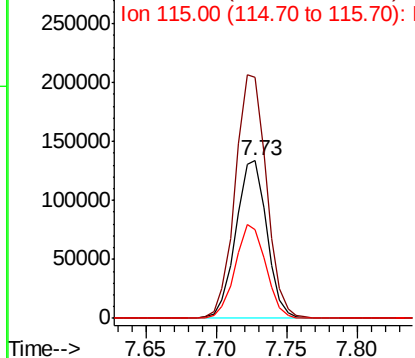

#5

2-Fluorophenol
Concen: 105.286 ng
RT: 5.32 min Scan# 379
Delta R.T. -0.01 min
Lab File: BM018665.D
Acq: 28 Jan 2019 15:43

Tgt Ion	Ratio	Lower	Upper
112	100		
64	54.3	46.5	69.7
63	30.0	25.2	37.8


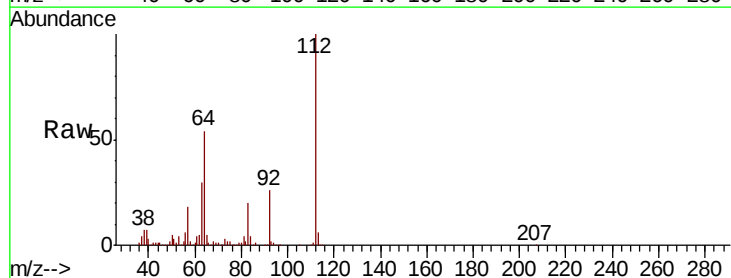



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

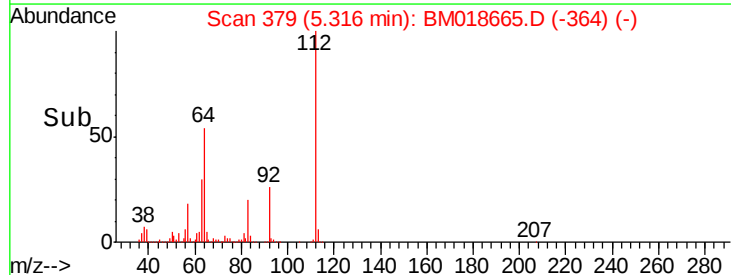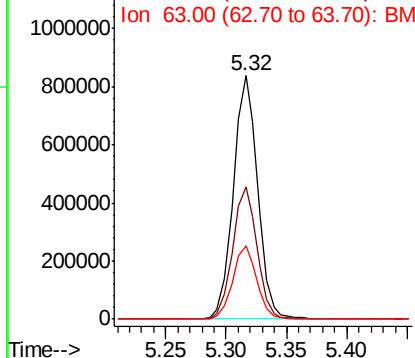



#7

Phenol-d6

Concen: 116.093 ng

RT: 6.90 min Scan# 648

Delta R.T. -0.01 min

Lab File: BM018665.D

Acq: 28 Jan 2019 15:43

Instrument :


BNA_F

ClientSampled :

GEN-1

Tot Ion: 99 Resp: 1646222

Ion	Ratio	Lower	Upper
99	100		
42	19.7	17.3	25.9
71	35.9	28.0	42.0



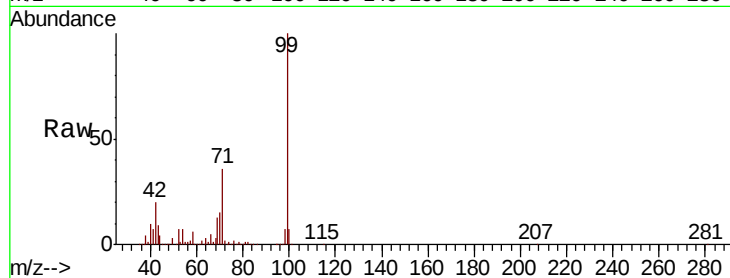


Abundance

Ion 99.00 (98.70 to 99.70): BM018466.D (-646) (-)

Ion 42.00 (41.70 to 42.70): BM018466.D (-646) (-)

Ion 71.00 (70.70 to 71.70): BM018466.D (-646) (-)

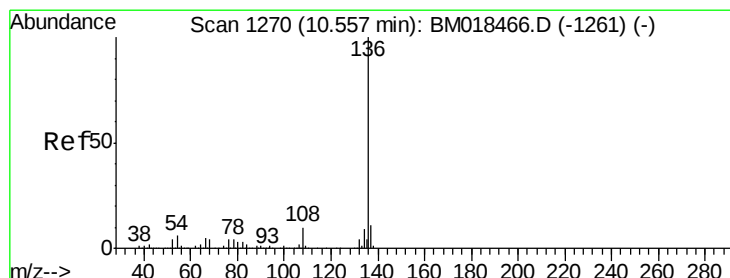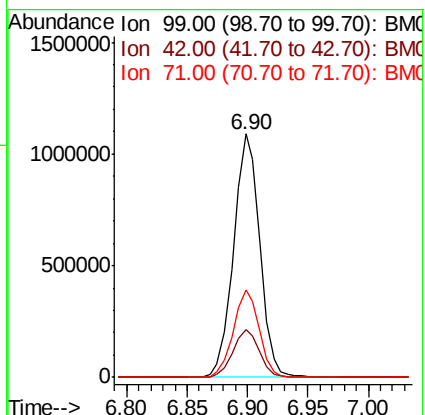

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.52 min Scan# 1263


Delta R.T. -0.01 min

Lab File: BM018665.D

Acq: 28 Jan 2019 15:43

Tgt Ion: 136 Resp: 816095

Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.5	12.7
54	6.2	6.0	9.0
68	4.6	4.5	6.7

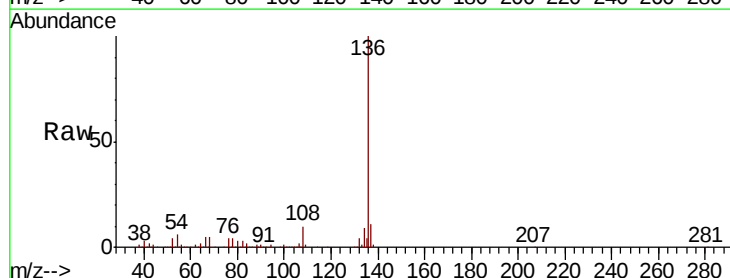



Abundance

Ion 136.00 (135.70 to 136.70): BM018466.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM018466.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM018466.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM018466.D (-1261) (-)


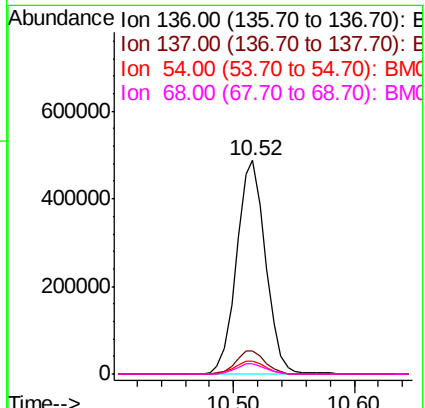





#23
Nitrobenzene-d5
Concen: 74.384 ng
RT: 8.89 min Scan# 987
Delta R.T. -0.01 min
Lab File: BM018665.D
Acq: 28 Jan 2019 15:43




Instrument :
BNA_F
ClientSampled :
GEN-1


Tot Ion: 82 Resp: 1047154
Ion Ratio Lower Upper
82 100
128 47.7 36.3 54.5
54 49.2 41.7 62.5

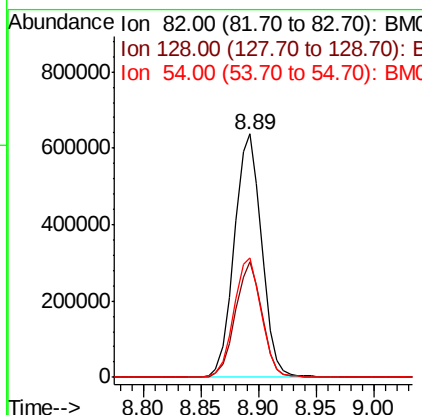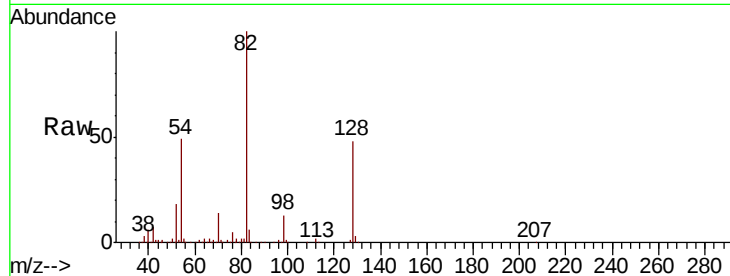

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.37 min Scan# 1919
Delta R.T. -0.01 min
Lab File: BM018665.D
Acq: 28 Jan 2019 15:43

Tgt Ion: 164 Resp: 460181
Ion Ratio Lower Upper
164 100
162 102.4 83.0 124.4
160 45.7 37.1 55.7

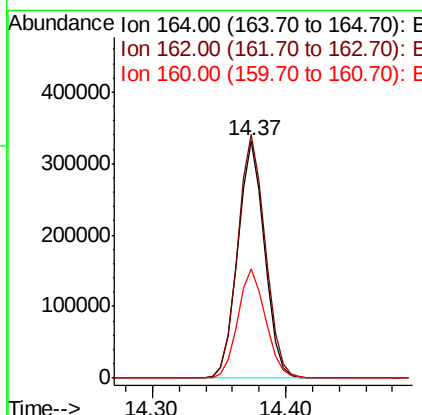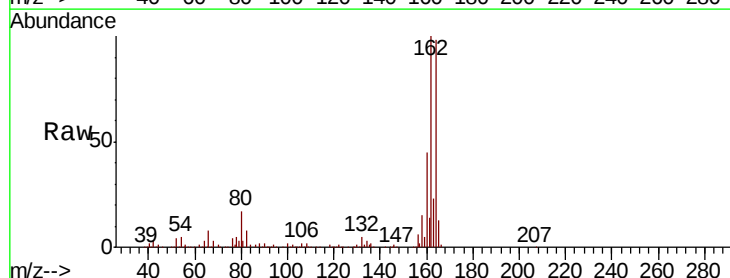




#42
 2,4,6-Tribromophenol
 Concen: 103.305 ng
 RT: 15.87 min Scan# 2173
 Delta R.T. -0.02 min
 Lab File: BM018665.D
 Acq: 28 Jan 2019 15:43

Instrument :
 BNA_F
 ClientSampled :
 GEN-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.2	77.6	116.4
141	38.4	31.7	47.5



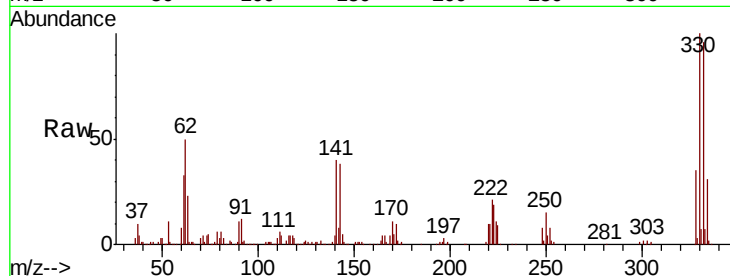


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

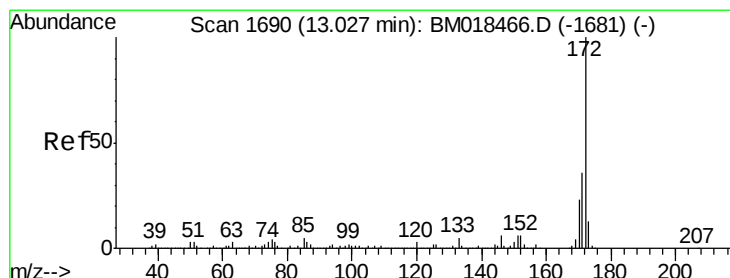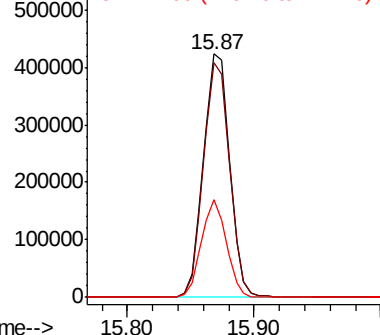

#45
 2-Fluorobiphenyl
 Concen: 75.066 ng
 RT: 12.99 min Scan# 1684
 Delta R.T. -0.01 min
 Lab File: BM018665.D
 Acq: 28 Jan 2019 15:43

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.6	28.2	42.4
170	23.3	18.9	28.3


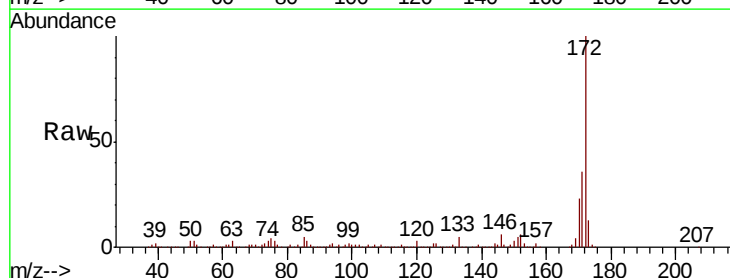



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

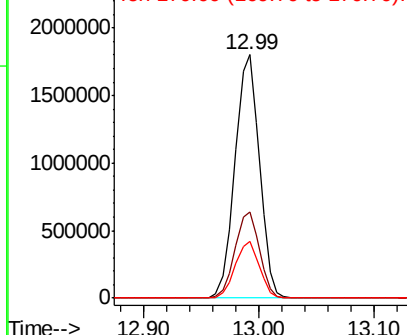



#50

Dimethylphthalate

Concen: 3.943 ng

RT: 13.84 min Scan# 1828

Delta R.T. -0.01 min

Lab File: BM018665.D

Acq: 28 Jan 2019 15:43

Instrument :

BNA_F

ClientSampleId :

GEN-1


Tot Ion:163 Resp: 149033

Ion Ratio Lower Upper

163 100

194 4.0 3.0 4.6




164 10.1 7.8 11.8

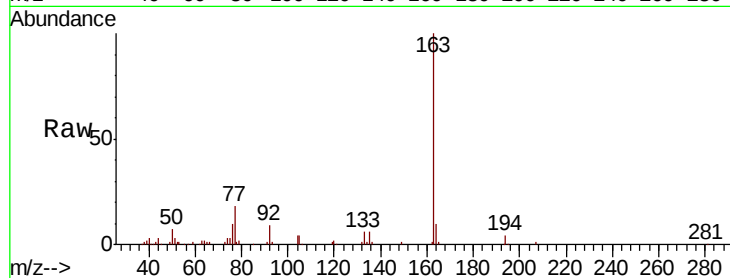

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

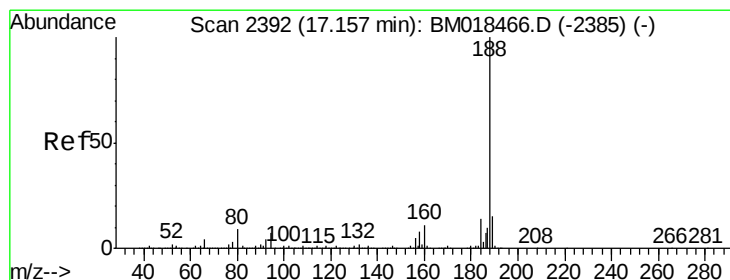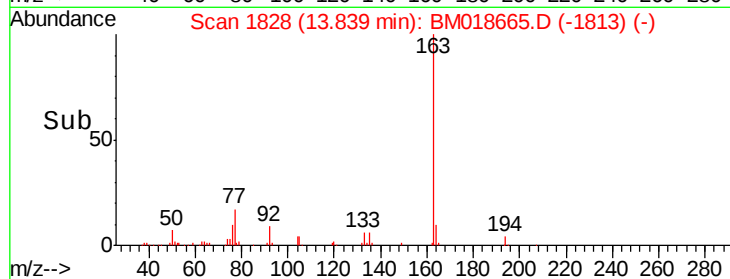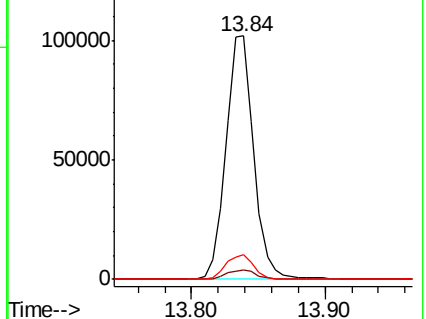

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.13 min Scan# 2387

Delta R.T. -0.01 min

Lab File: BM018665.D

Acq: 28 Jan 2019 15:43


Tgt Ion:188 Resp: 1034022

Ion Ratio Lower Upper

188 100

94 6.9 7.1 10.7#



80 8.1 7.6 11.4

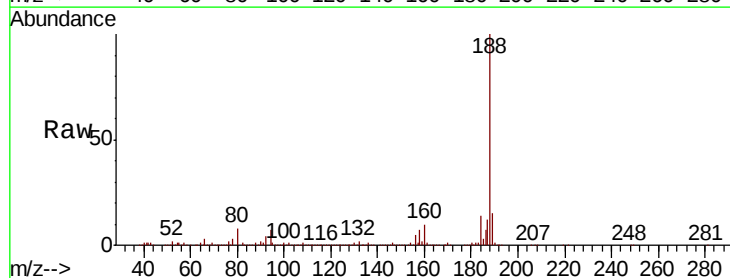


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0




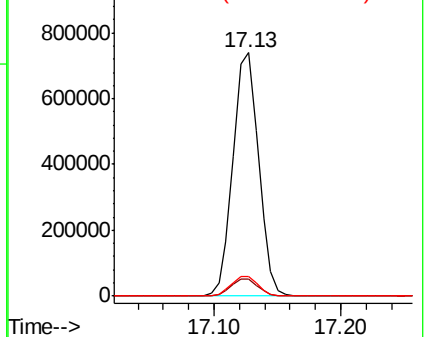


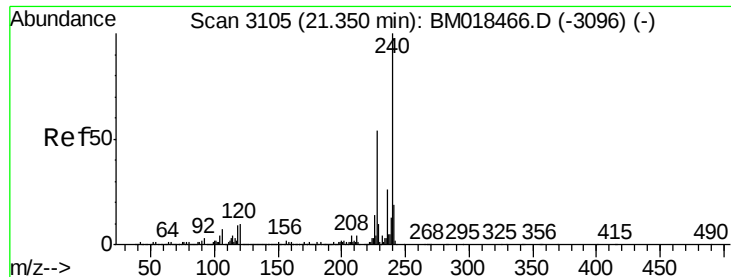

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.32 min Scan# 3100
 Delta R.T. -0.01 min
 Lab File: BM018665.D
 Acq: 28 Jan 2019 15:43




Instrument :
 BNA_F
 ClientSampleID :
 GEN-1


Tot Ion:240 Resp: 1104454
 Ion Ratio Lower Upper
 240 100
 120 9.1 8.4 12.6
 236 26.1 20.7 31.1

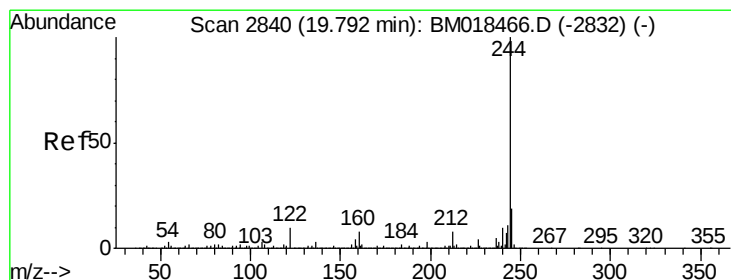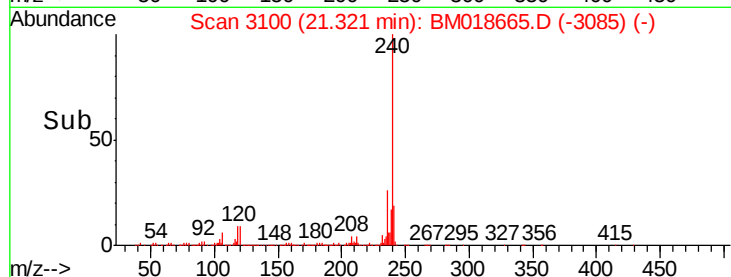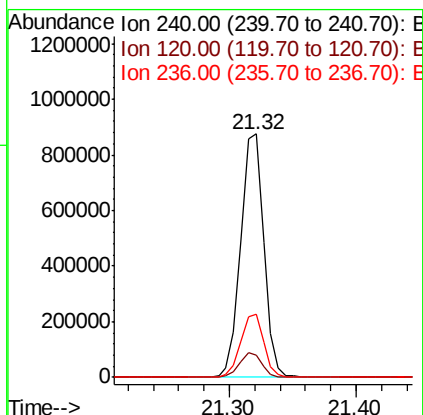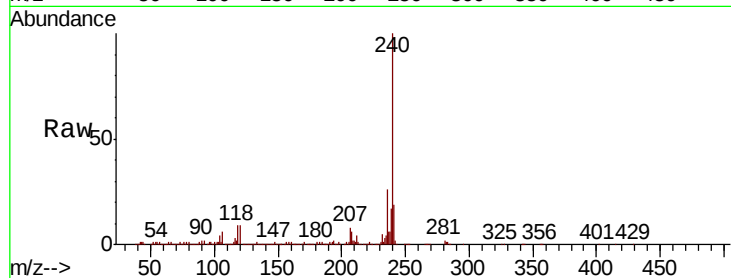

#79
 Terphenyl-d14
 Concen: 76.171 ng
 RT: 19.76 min Scan# 2835
 Delta R.T. -0.01 min
 Lab File: BM018665.D
 Acq: 28 Jan 2019 15:43

Tgt Ion:244 Resp: 3990782
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.9 8.9
 122 8.6 9.0 13.4#

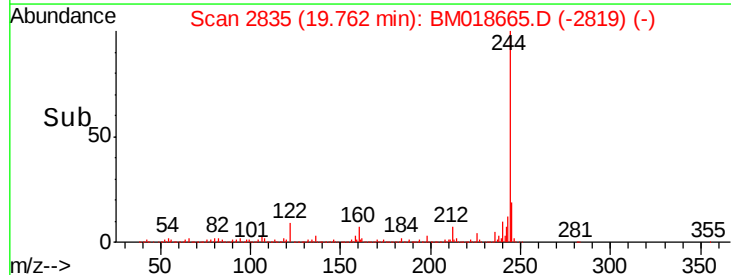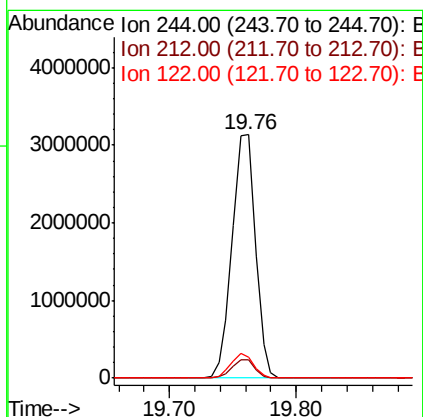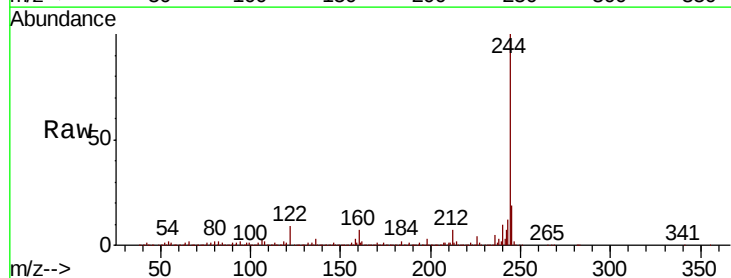

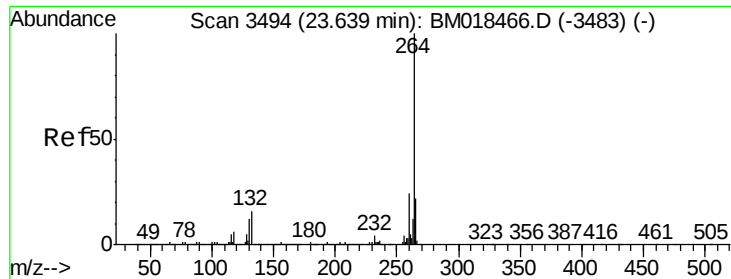

#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.59 min Scan# 3485
Delta R.T. -0.02 min
Lab File: BM018665.D
Acq: 28 Jan 2019 15:43

Instrument :
BNA_F
ClientSampleId :
GEN-1

Tot Ion:264 Resp: 1120911

Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.9	28.3
265	21.5	16.8	25.2

