
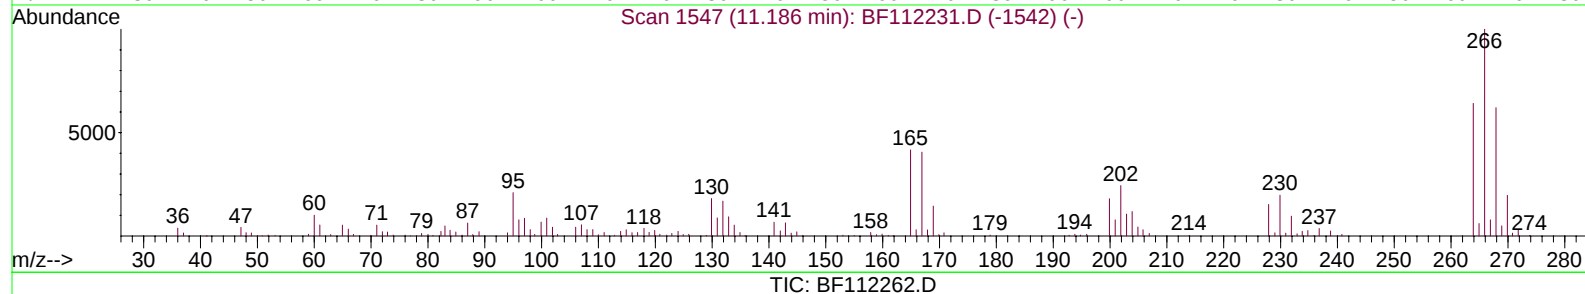
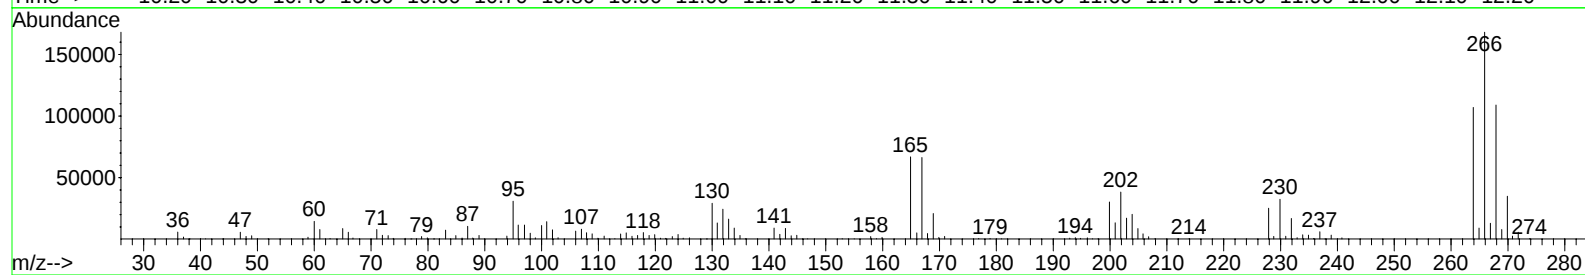


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012819\
Data File : BF112262.D
Acq On : 28 Jan 2019 9:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 15:40:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

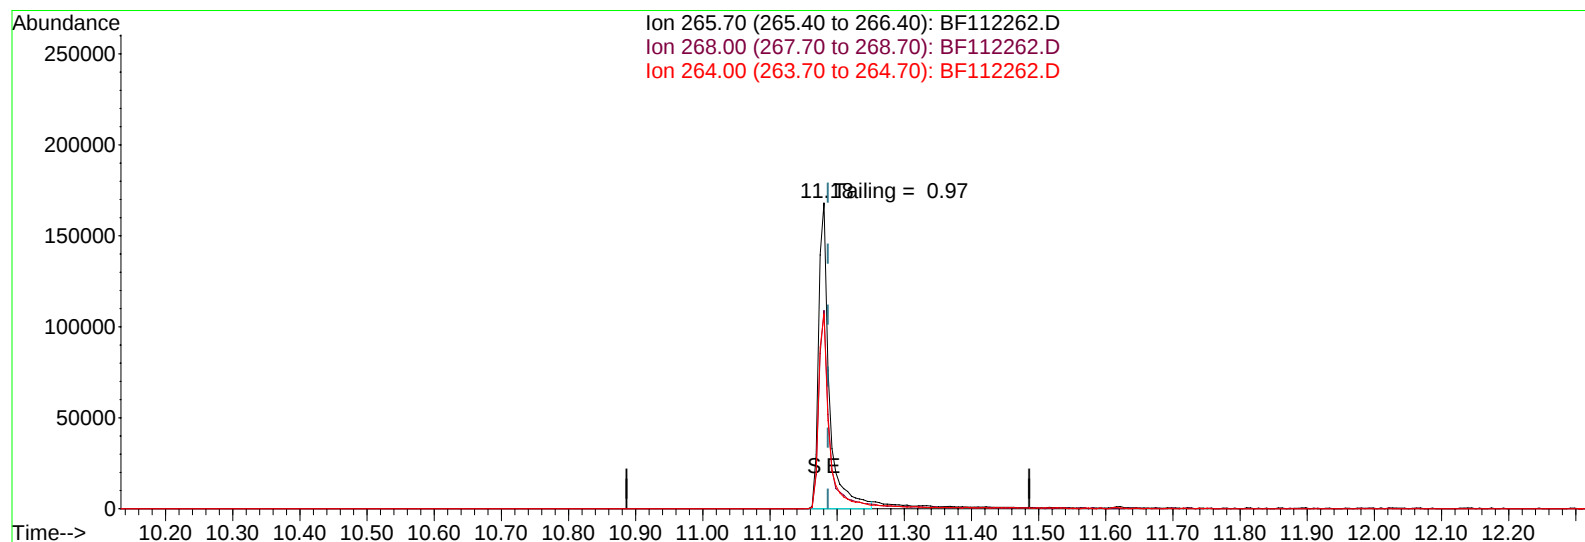

(70) Pentachlorophenol (C)




11.180min (-0.006) 16731.05ng m

response 187957

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.84
264.00	63.60	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012819\
 Data File : BF112262.D
 Acq On : 28 Jan 2019 9:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 15:40:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

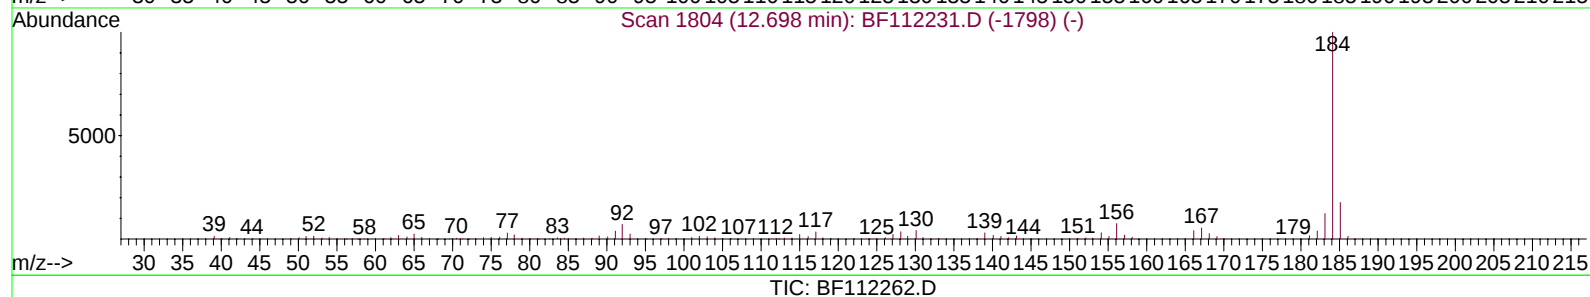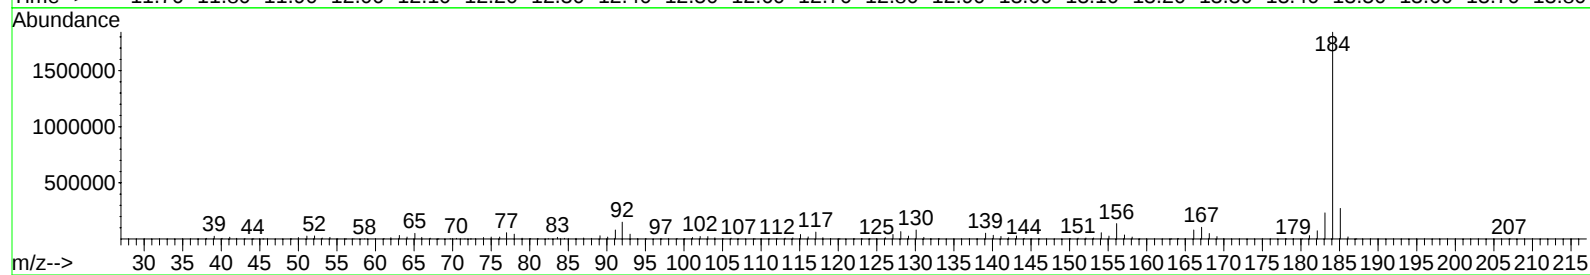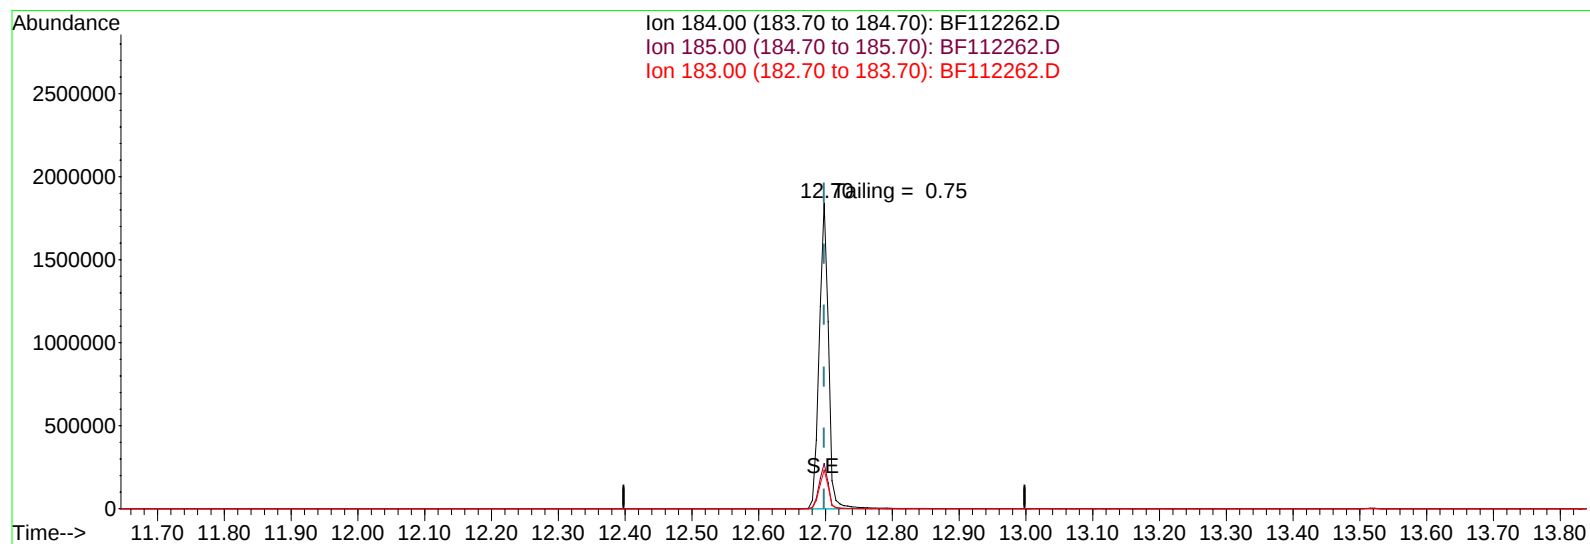

(77) Benzidine

12.698min (+0.000) 16559.30ng

response 1770206

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.83
183.00	12.50	12.66
0.00	0.00	0.00