

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012819\
 Data File : BF112271.D
 Acq On : 28 Jan 2019 13:40
 Operator : JU/SJ
 Sample : K1258-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-AA01-BB01-AA01A-AA0

Quant Time: Jan 28 14:16:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	201835	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	809329	20.00	ng	0.00
39) Acenaphthene-d10	9.87	164	408438	20.00	ng	-0.01
64) Phenanthrene-d10	11.36	188	817017	20.00	ng	0.00
76) Chrysene-d12	14.00	240	641854	20.00	ng	0.00
87) Perylene-d12	15.47	264	496762	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	1311672	138.04	ng	0.00
7) Phenol-d6	6.49	99	1650164	124.98	ng	0.00
23) Nitrobenzene-d5	7.40	82	1058281	75.34	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	580100	122.02	ng	-0.01
45) 2-Fluorobiphenyl	9.20	172	2149935	74.45	ng	0.00
79) Terphenyl-d14	12.94	244	2328904	68.34	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.59	163	114950	3.622	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012819\
Data File : BF112271.D
Acq On : 28 Jan 2019 13:40
Operator : JU/SJ
Sample : K1258-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-AA01-BB01-AA01A-AA0

Quant Time: Jan 28 14:16:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

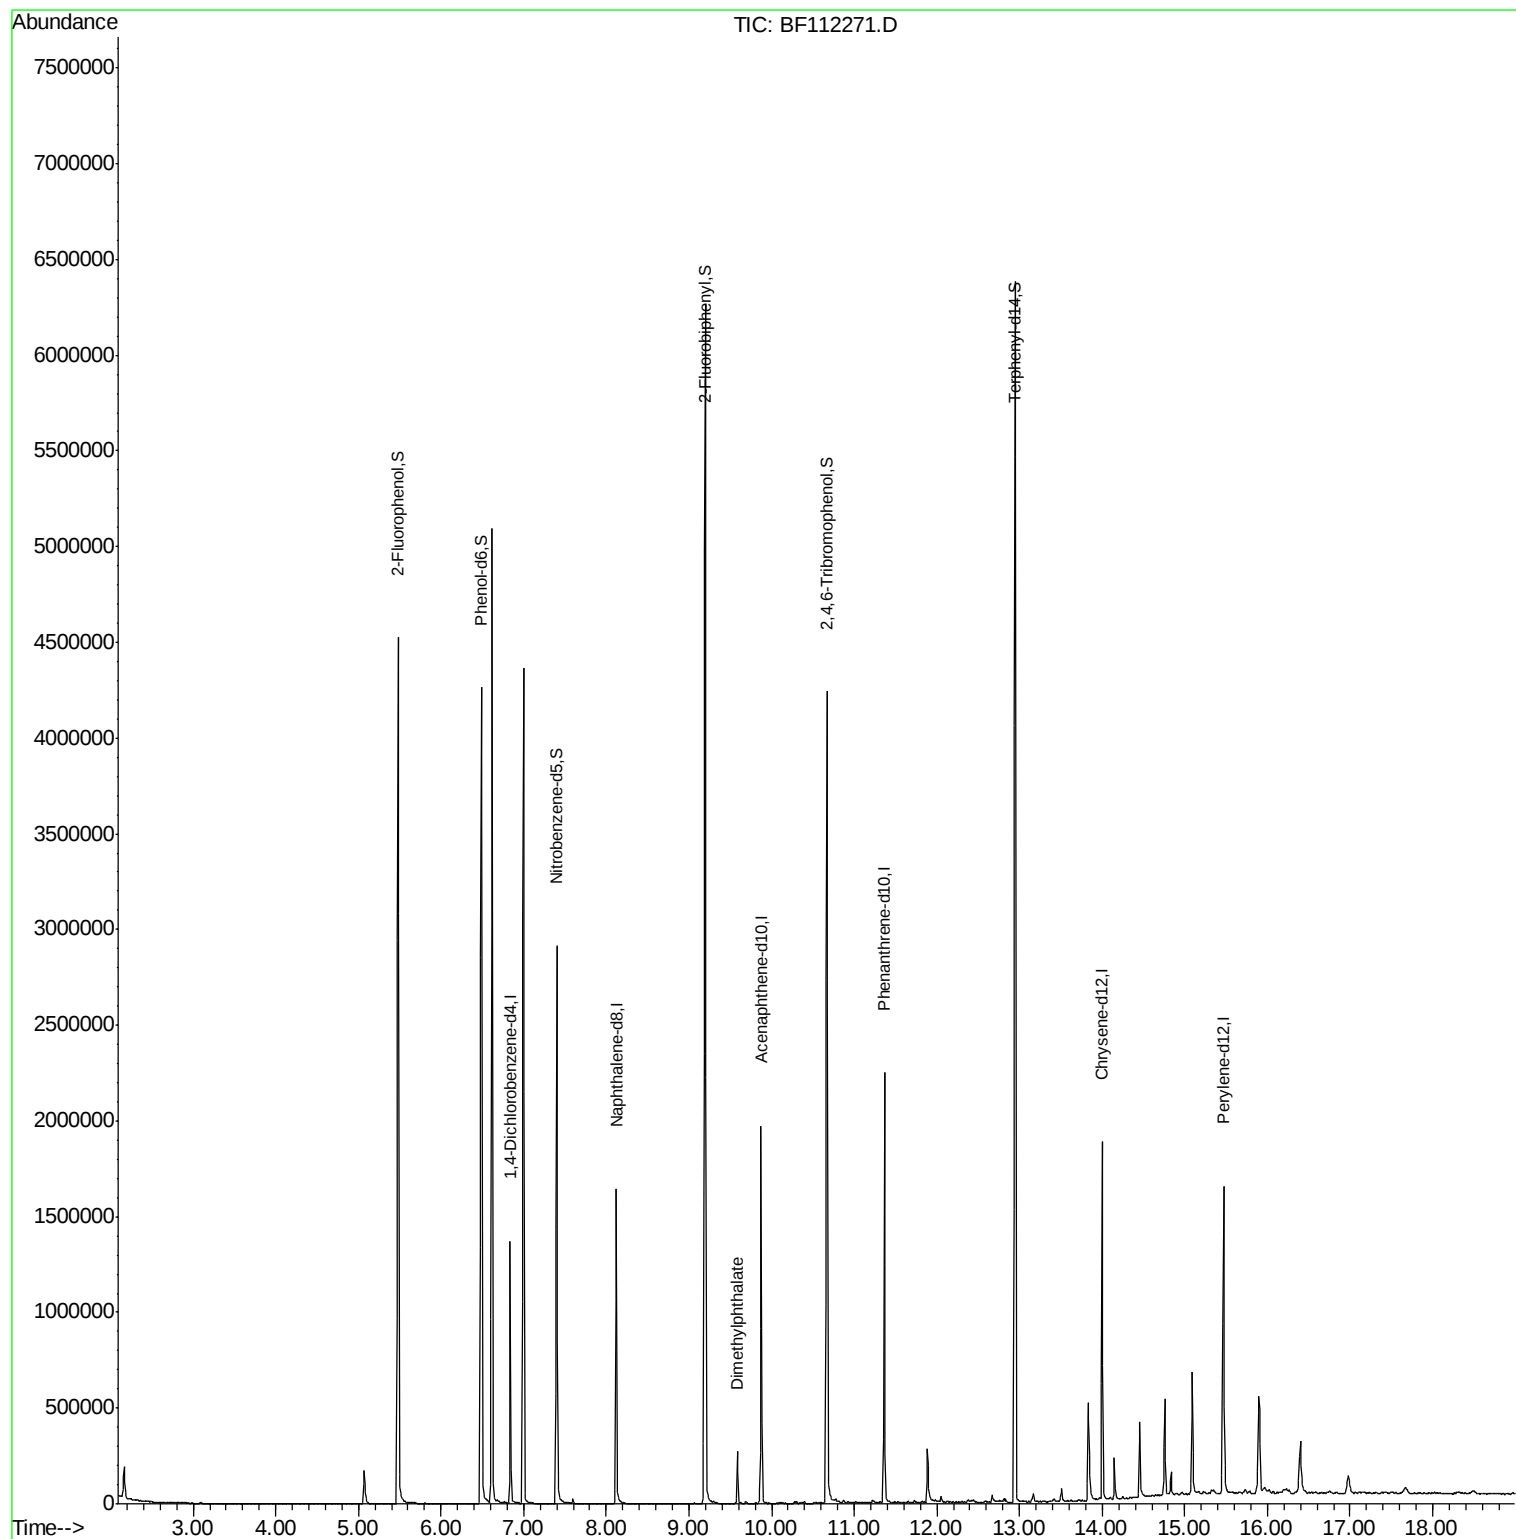

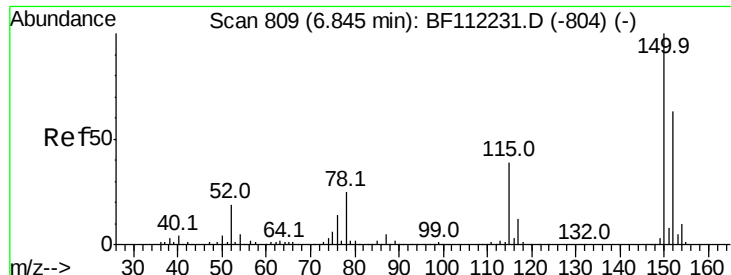


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.84 min Scan# 808
Delta R.T. -0.01 min
Lab File: BF112271.D
Acq: 28 Jan 2019 13:40

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-AA01-BB01-AA01A-AA0

Tot Ion:152 Resp: 201835
Ion Ratio Lower Upper
152 100
150 154.0 127.4 191.0
115 58.1 45.5 68.3

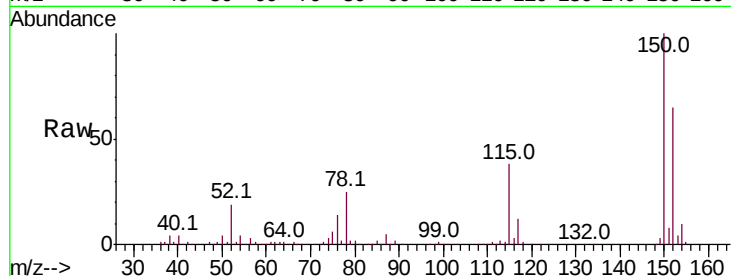


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

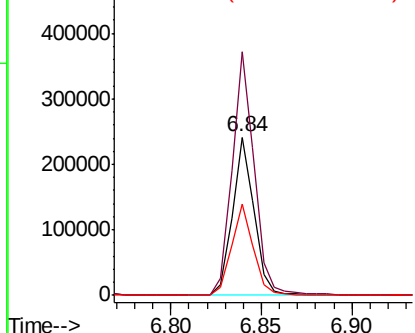



#5


2-Fluorophenol
Concen: 138.037 ng
RT: 5.48 min Scan# 577
Delta R.T. -0.00 min
Lab File: BF112271.D
Acq: 28 Jan 2019 13:40

Tgt Ion:112 Resp: 1311672
Ion Ratio Lower Upper
112 100
64 57.4 45.7 68.5
63 31.0 23.6 35.4

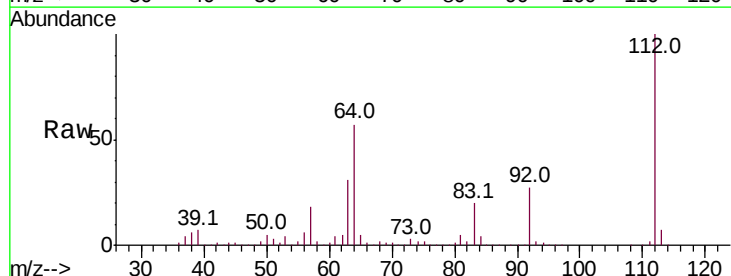

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

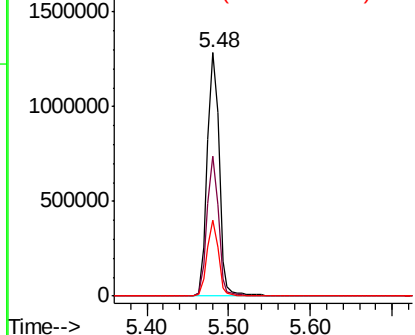

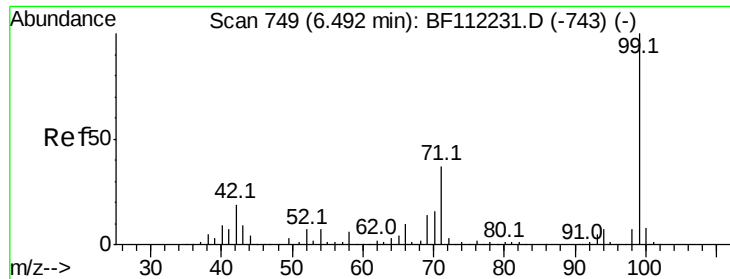

#7

Phenol-d6

Concen: 124.975 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF112271.D

Acq: 28 Jan 2019 13:40

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-AA01-BB01-AA01A-AA0


Tot Ion: 99 Resp: 1650164

Ion Ratio Lower Upper




99 100

42 19.5 15.1 22.7

71 37.1 26.9 40.3

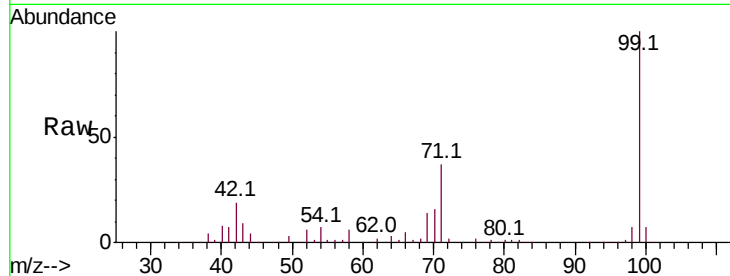

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

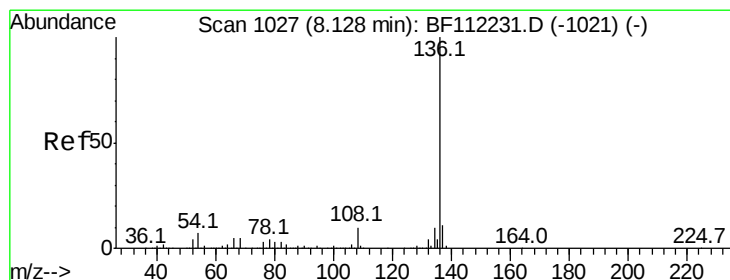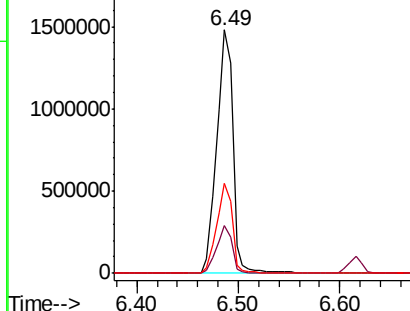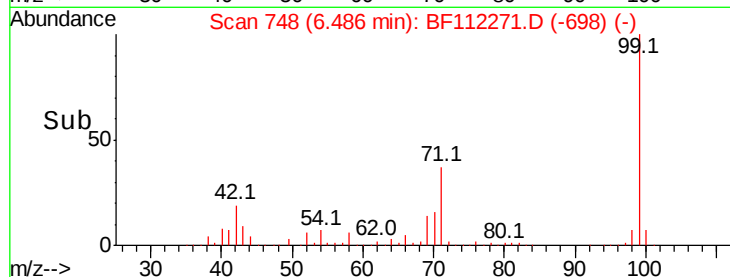

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1026

Delta R.T. -0.01 min

Lab File: BF112271.D

Acq: 28 Jan 2019 13:40

Tgt Ion: 136 Resp: 809329


Ion Ratio Lower Upper

136 100



137 10.8 9.1 13.7


54 6.4 5.9 8.9

68 5.3 5.1 7.7

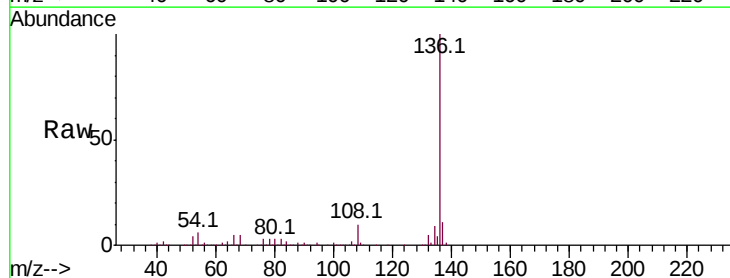

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

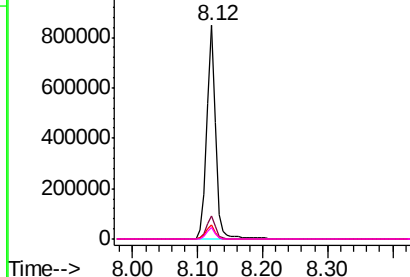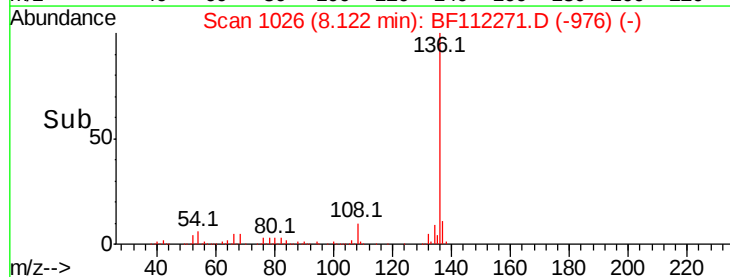


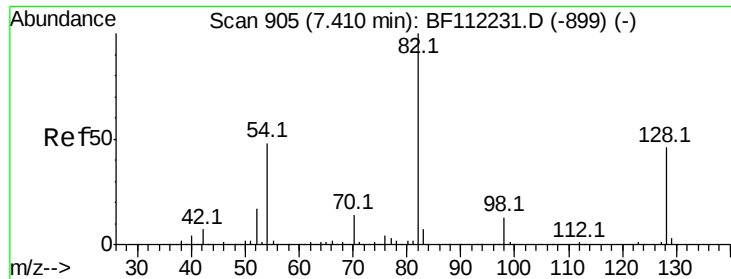




#23
Nitrobenzene-d5
Concen: 75.344 ng
RT: 7.40 min Scan# 904
Delta R.T. -0.01 min
Lab File: BF112271.D
Acq: 28 Jan 2019 13:40

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-AA01-BB01-AA01A-AA0

Tot Ion: 82 Resp: 1058281
Ion Ratio Lower Upper
82 100
128 48.0 37.8 56.8
54 48.7 39.7 59.5

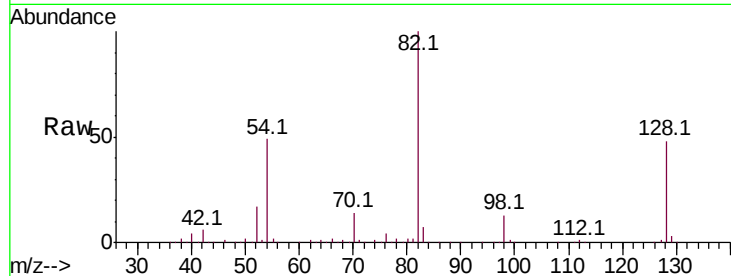


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

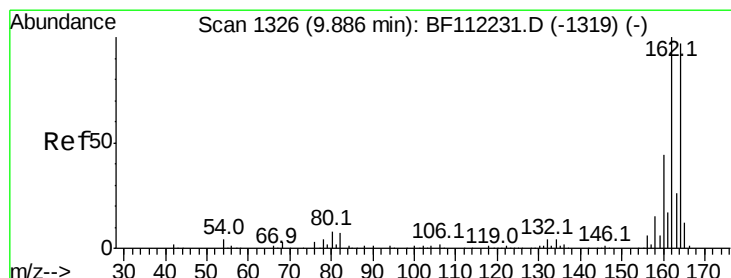
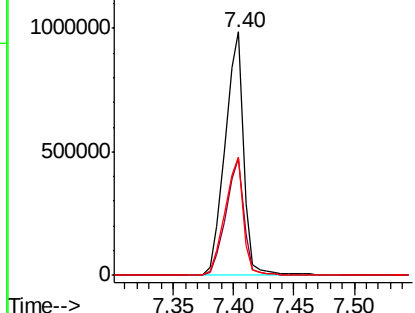



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.87 min Scan# 1324
Delta R.T. -0.01 min
Lab File: BF112271.D
Acq: 28 Jan 2019 13:40

Tgt Ion:164 Resp: 408438
Ion Ratio Lower Upper
164 100
162 104.4 82.2 123.4
160 47.0 36.2 54.4



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

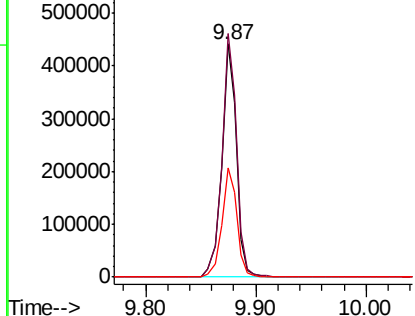


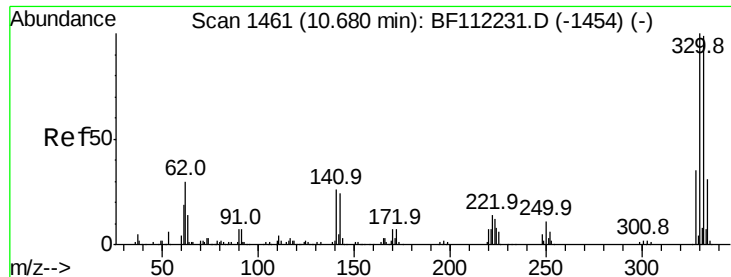




#42
 2,4,6-Tribromophenol
 Concen: 122.021 ng
 RT: 10.67 min Scan# 1459
 Delta R.T. -0.01 min
 Lab File: BF112271.D
 Acq: 28 Jan 2019 13:40

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-AA01-BB01-AA01A-AA0

Tot Ion:330 Resp: 580100
 Ion Ratio Lower Upper
 330 100
 332 95.3 76.6 114.8
 141 31.4 24.3 36.5

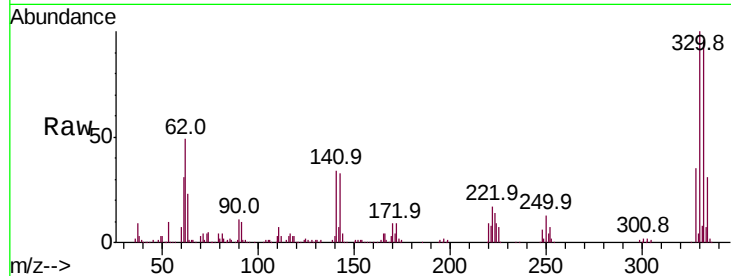


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


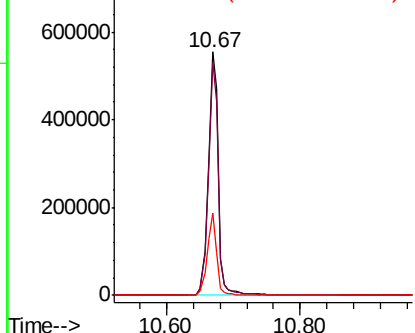



#45
 2-Fluorobiphenyl
 Concen: 74.448 ng
 RT: 9.20 min Scan# 1209
 Delta R.T. -0.01 min
 Lab File: BF112271.D
 Acq: 28 Jan 2019 13:40

Tgt Ion:172 Resp: 2149935
 Ion Ratio Lower Upper
 172 100
 171 37.2 30.5 45.7
 170 24.8 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

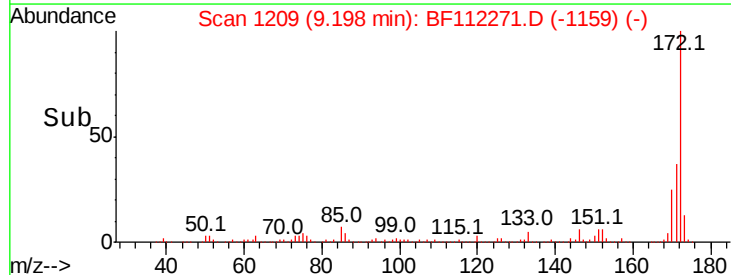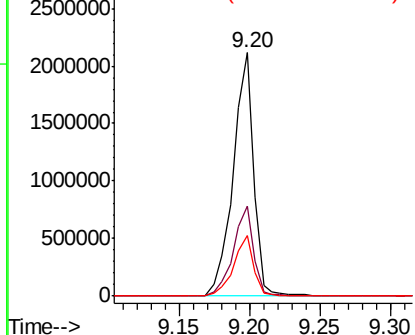



#50

Dimethylphthalate

Concen: 3.622 ng

RT: 9.59 min Scan# 1275

Delta R.T. -0.02 min

Lab File: BF112271.D

Acq: 28 Jan 2019 13:40

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-AA01-BB01-AA01A-AA0


Tot Ion:163 Resp: 114950

Ion Ratio Lower Upper

163 100

194 3.9 3.3 4.9




164 10.0 8.5 12.7



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

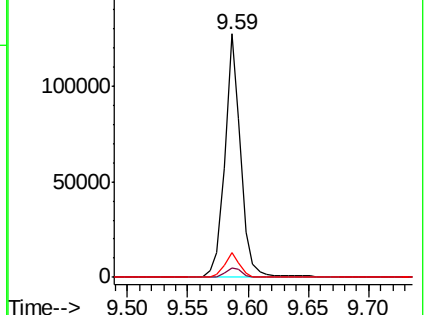

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.36 min Scan# 1577

Delta R.T. -0.01 min

Lab File: BF112271.D

Acq: 28 Jan 2019 13:40


Tgt Ion:188 Resp: 817017

Ion Ratio Lower Upper

188 100

94 9.0 8.2 12.2



80 9.8 8.9 13.3




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

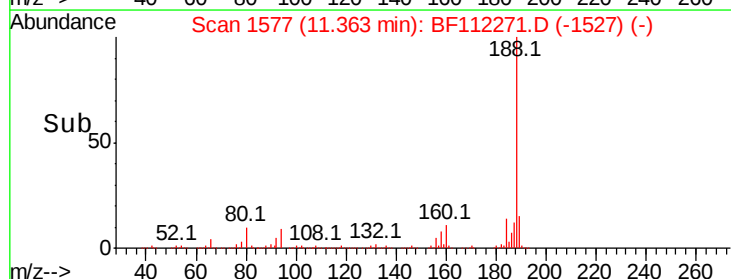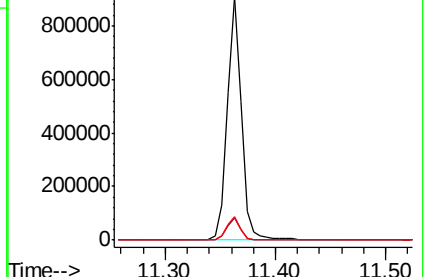



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.00 min Scan# 2026

Delta R.T. -0.01 min

Lab File: BF112271.D

Acq: 28 Jan 2019 13:40

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-AA01-BB01-AA01A-AA0


Tot Ion:240 Resp: 641854

Ion Ratio Lower Upper

240 100

120 10.1 9.0 13.6




236 25.6 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

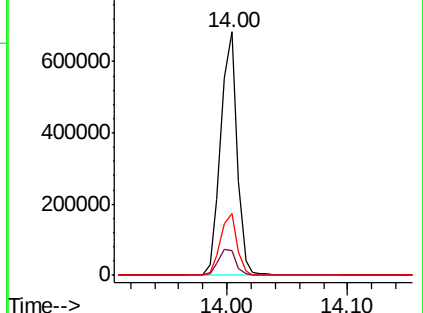

#79

Terphenyl-d14

Concen: 68.339 ng

RT: 12.94 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BF112271.D

Acq: 28 Jan 2019 13:40


Tgt Ion:244 Resp: 2328904

Ion Ratio Lower Upper

244 100

212 7.7 5.9 8.9



122 12.9 9.8 14.6




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

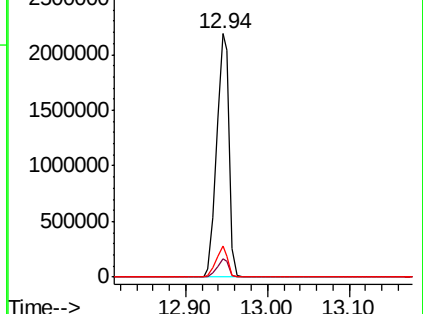


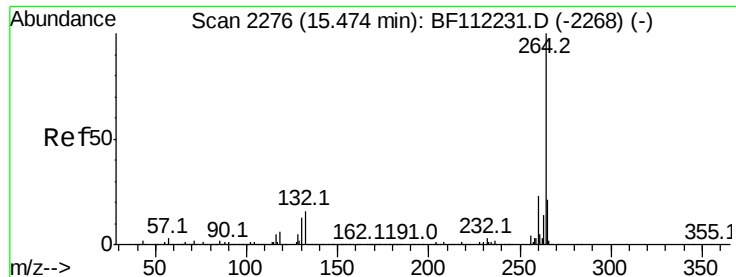

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.47 min Scan# 2275
 Delta R.T. -0.01 min
 Lab File: BF112271.D
 Acq: 28 Jan 2019 13:40

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-AA01-BB01-AA01A-AA0

Tot Ion:	264	Resp:	496762
Ion	Ratio	Lower	Upper
264	100		
260	22.9	18.2	27.2
265	21.6	17.0	25.4

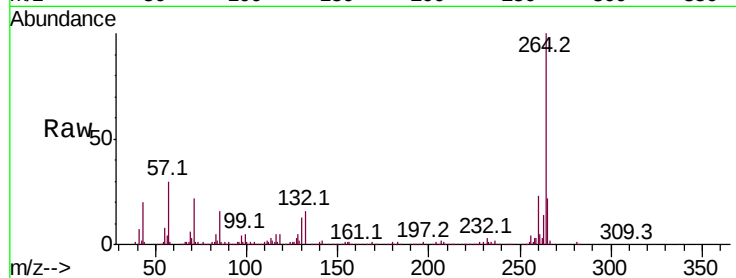

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

