


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012819\
Data File : BF112262.D
Acq On : 28 Jan 2019 9:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jan 28 10:38:18 2019

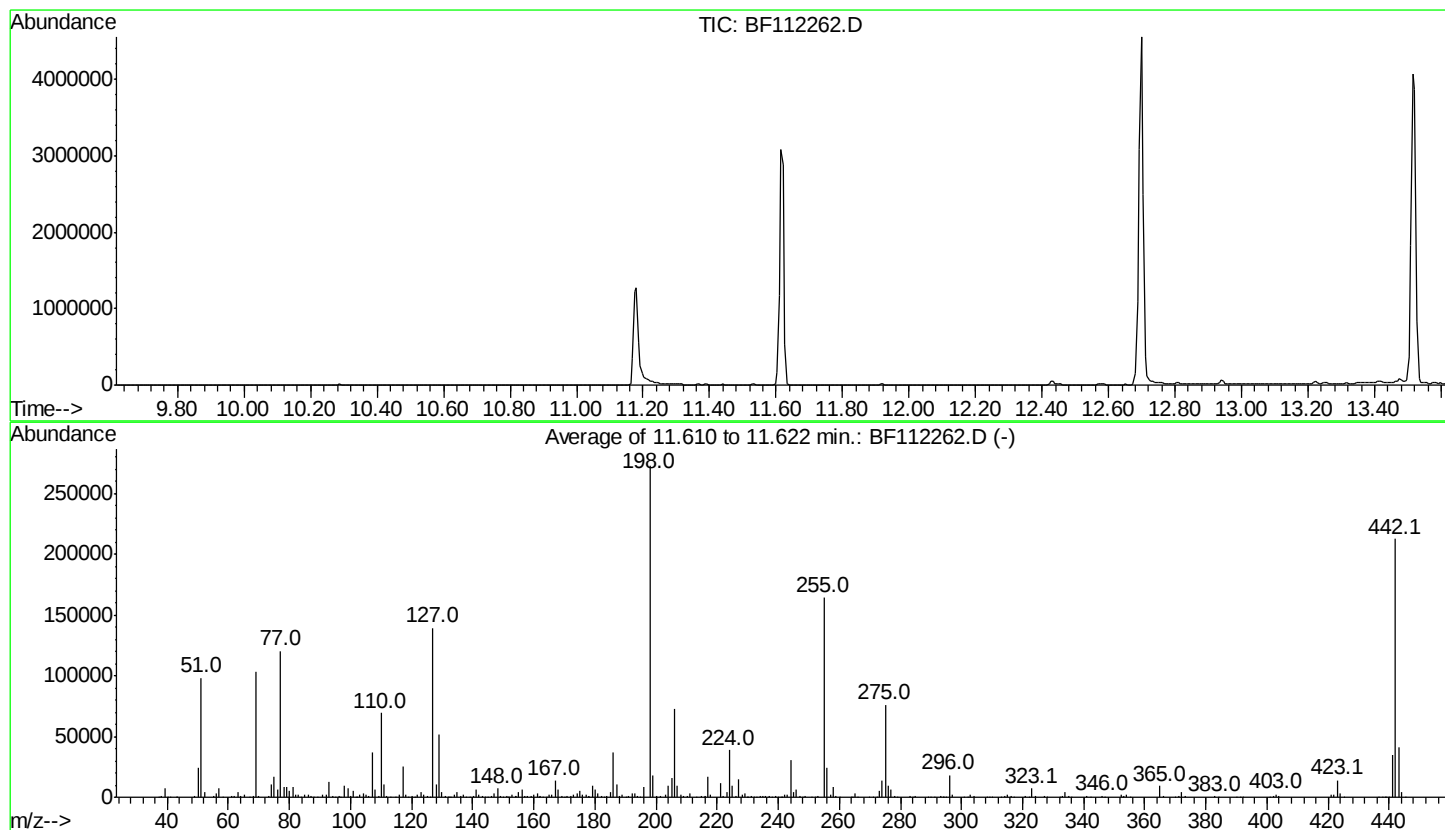

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	98373	PASS
68	69	0.00	2	1.5	1528	PASS
69	198	0.00	100	37.9	103562	PASS
70	69	0.00	2	0.7	730	PASS
127	198	10	80	51.0	139352	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	272981	PASS
199	198	5	9	6.7	18156	PASS
275	198	10	60	27.8	75944	PASS
365	198	1	100	3.4	9346	PASS
441	198	0.01	100	12.7	34620	PASS
442	198	50	100	77.9	212616	PASS
443	442	15	24	19.3	41068	PASS