
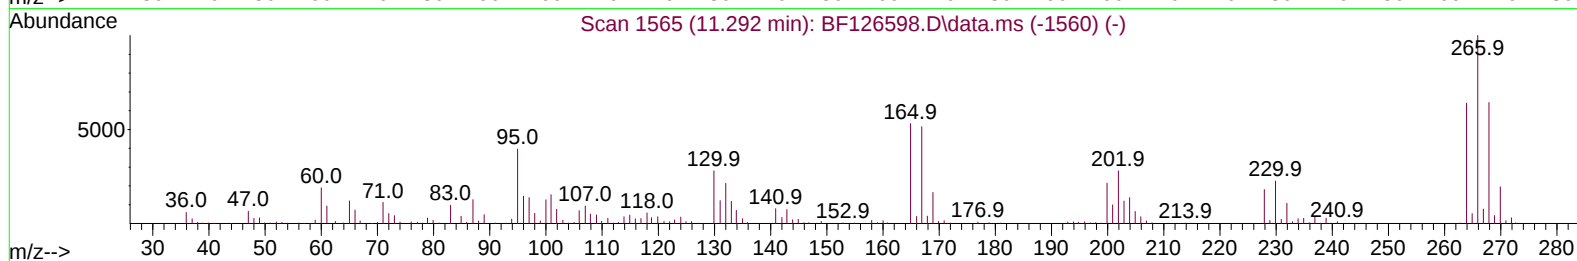
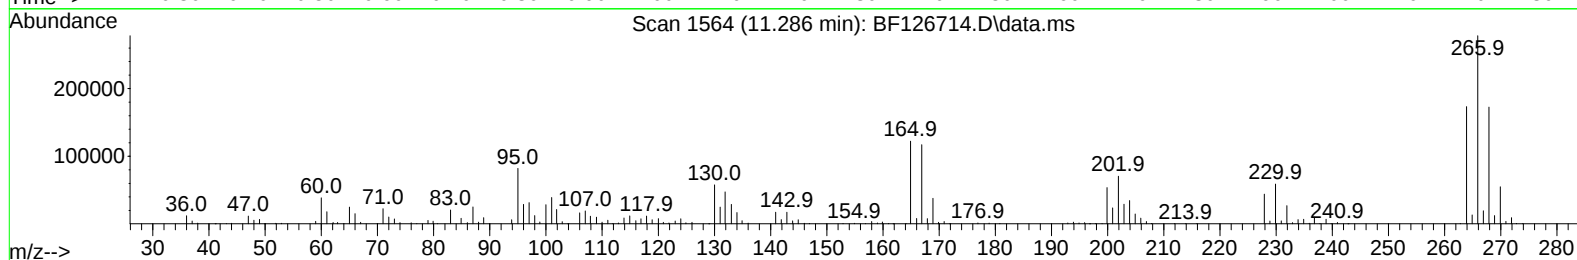


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126714.D
Acq On : 28 Jan 2022 13:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 04:02:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration

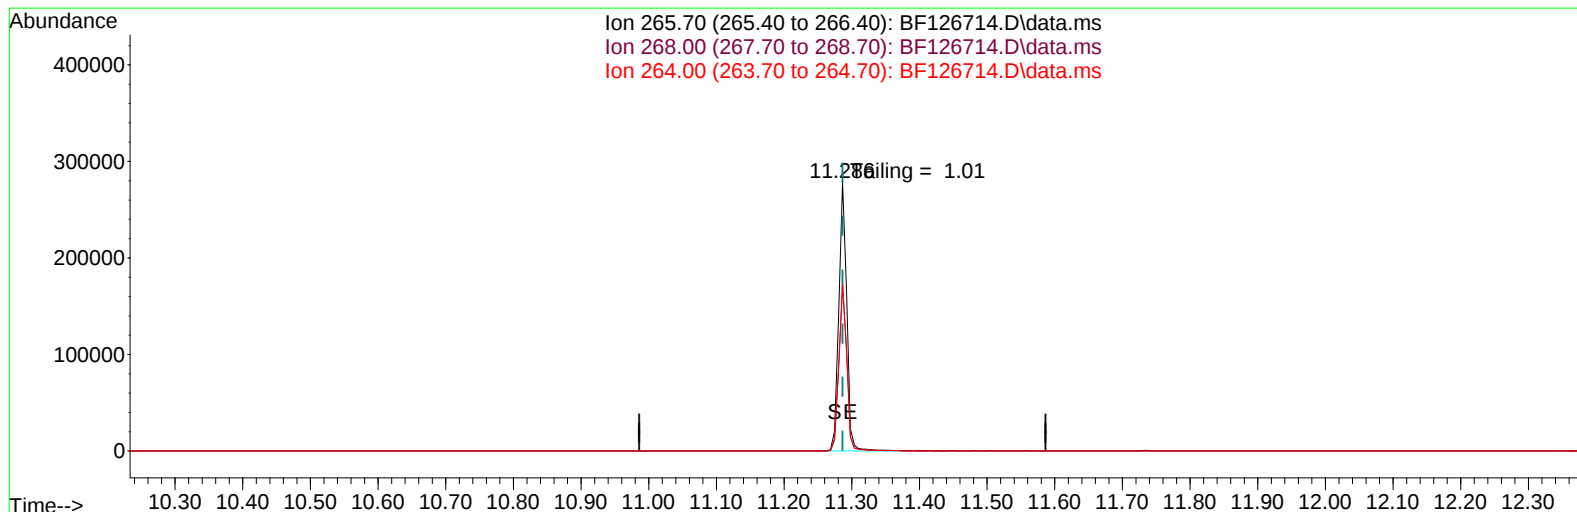

TIC: BF126714.D\data.ms

(70) Pentachlorophenol (C)




11.286min (+ 0.000) 35096.41 ng

response **228365**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.09
264.00	63.00	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126714.D
Acq On : 28 Jan 2022 13:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 04:02:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration

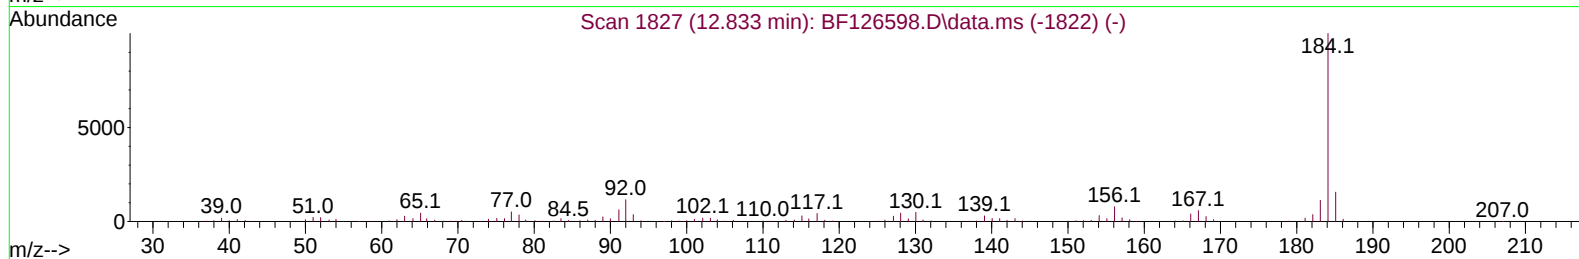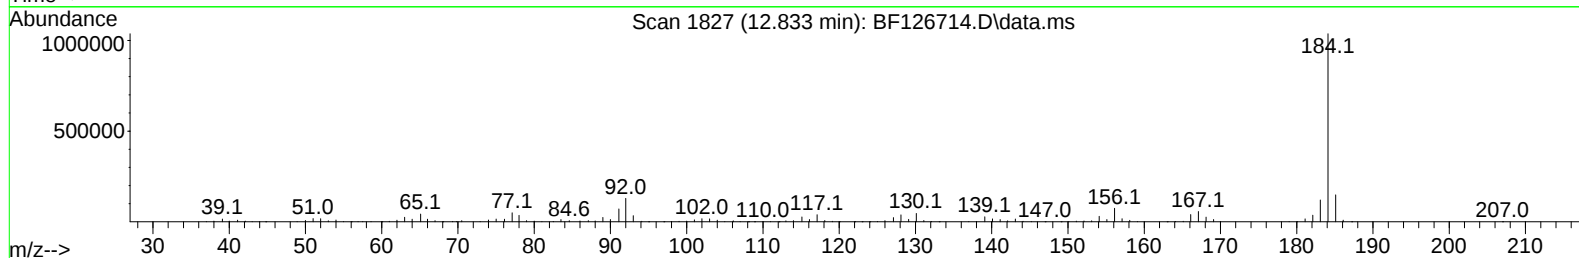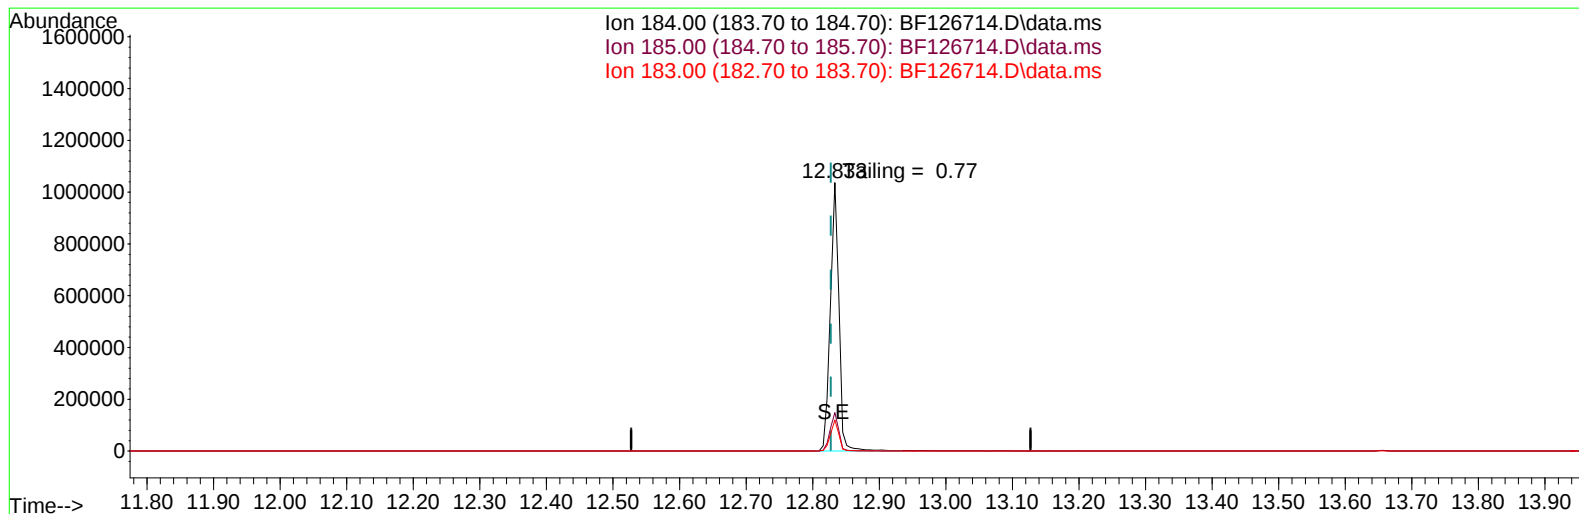

TIC: BF126714.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 0.00 ng

response 940708

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.30
183.00	10.20	11.58
0.00	0.00	0.00