

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
 Data File : BF126716.D
 Acq On : 28 Jan 2022 15:10
 Operator : CG/JU
 Sample : PB142340BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 2

Instrument :
 BNA_F
 ClientSampleId :
 PB142340BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.346	35	44	49	rVB	67980	99674	1.61%	0.209%
2	5.587	589	595	598	rBV	5268904	5667452	91.36%	11.900%
3	6.575	757	763	766	rBV	5007437	5955174	96.00%	12.504%
4	6.957	824	828	831	rBV	2444013	2066557	33.31%	4.339%
5	7.522	918	924	927	rBV	3440926	3945560	63.61%	8.285%
6	8.239	1040	1046	1049	rBV	3055234	2791910	45.01%	5.862%
7	9.316	1223	1229	1232	rBV	6314514	6002698	96.77%	12.604%
8	9.998	1340	1345	1348	rBV	3753336	3229644	52.06%	6.781%
9	10.786	1475	1479	1483	rBV	3666003	3751284	60.47%	7.877%
10	11.492	1595	1599	1602	rBV	3811851	3231509	52.09%	6.785%
11	13.086	1864	1870	1873	rBV	5983435	6203131	100.00%	13.025%
12	14.139	2045	2049	2053	rBV	2851079	2508313	40.44%	5.267%
13	15.662	2301	2308	2316	rBV	1476594	1950441	31.44%	4.095%
14	16.698	2478	2484	2489	rBV2	34598	69745	1.12%	0.146%
15	17.774	2657	2667	2678	rVB5	39932	152619	2.46%	0.320%




Sum of corrected areas: 47625711

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126716.D
Acq On : 28 Jan 2022 15:10
Operator : CG/JU
Sample : PB142340BL
Misc :
ALS Vial : 3 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
PB142340BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

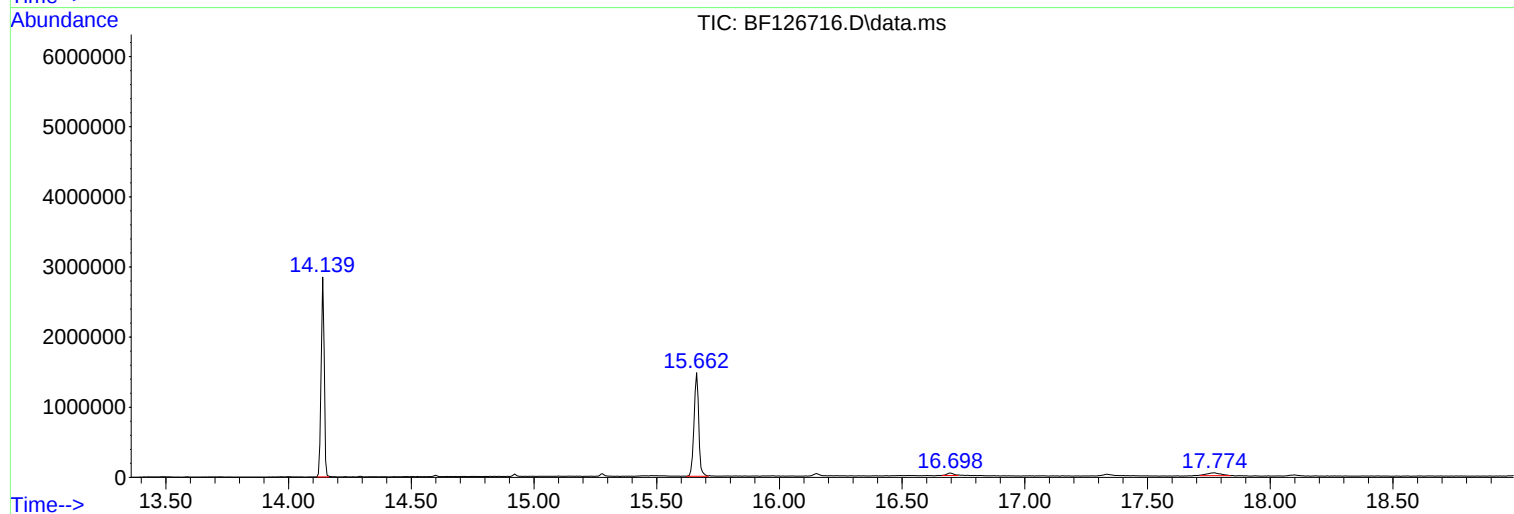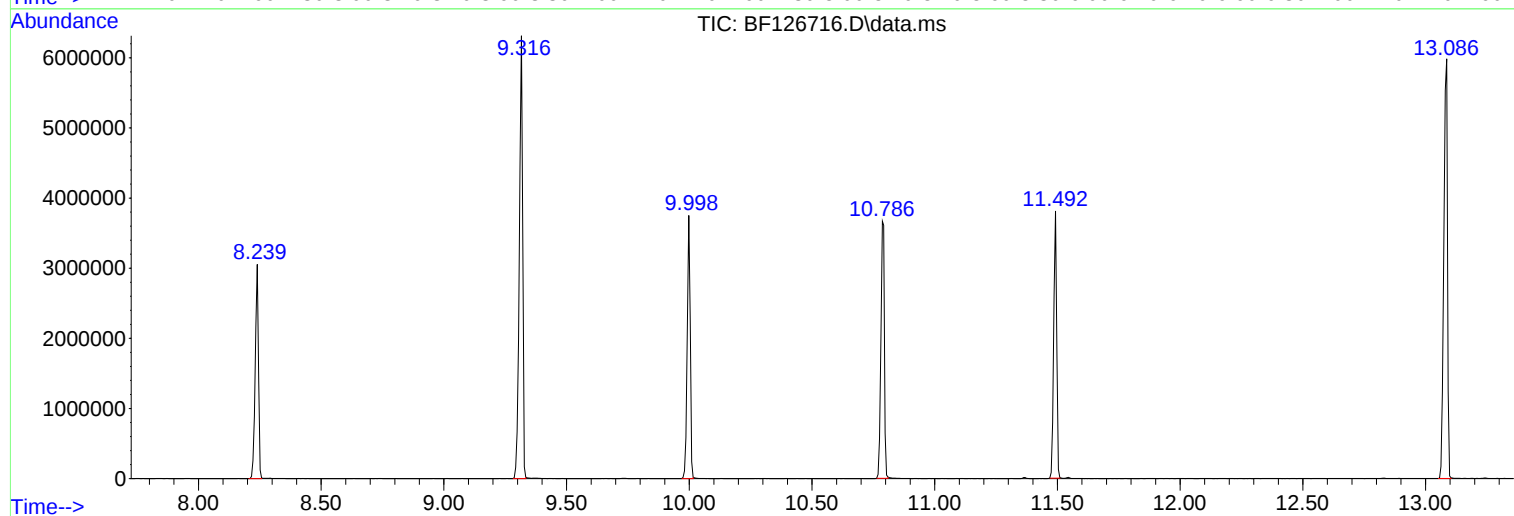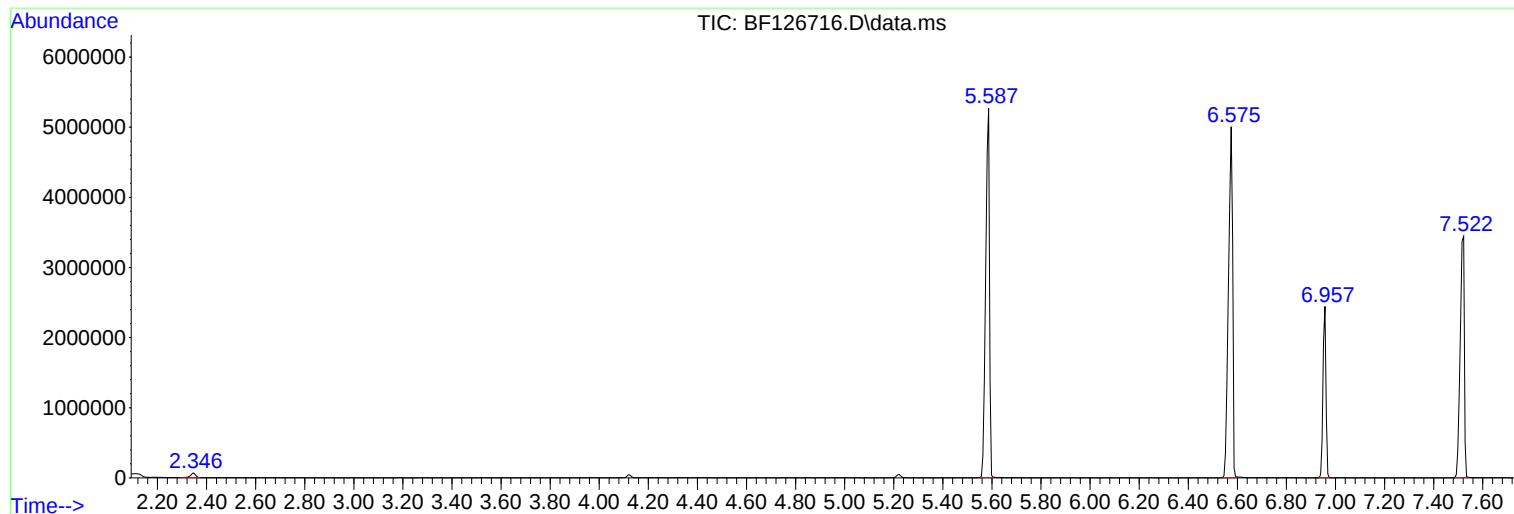

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126716.D
Acq On : 28 Jan 2022 15:10
Operator : CG/JU
Sample : PB142340BL
Misc :
ALS Vial : 3 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
PB142340BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126716.D
Acq On : 28 Jan 2022 15:10
Operator : CG/JU
Sample : PB142340BL
Misc :
ALS Vial : 3 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
PB142340BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------