

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
 Data File : BF126739.D
 Acq On : 29 Jan 2022 01:36
 Operator : CG/JU
 Sample : N1314-01 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-012722

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	20	25	33	rVB	112976	146519	12.69%	1.070%
2	4.069	333	337	343	rVB	19857	24690	2.14%	0.180%
3	5.563	587	591	595	rBV	611304	524242	45.42%	3.827%
4	6.563	758	761	766	rBV	601570	499616	43.29%	3.647%
5	6.781	795	798	803	rBV3	19709	21446	1.86%	0.157%
6	6.957	824	828	832	rVB	1247980	974850	84.46%	7.116%
7	7.228	868	874	876	rBV3	16552	20389	1.77%	0.149%
8	7.486	912	918	920	rBV4	20210	25228	2.19%	0.184%
9	7.516	920	923	926	rVV	370862	317338	27.49%	2.317%
10	7.545	926	928	932	rVB	48074	41009	3.55%	0.299%
11	7.598	932	937	941	rBV6	18147	30912	2.68%	0.226%
12	7.651	941	946	950	rVV4	10461	18473	1.60%	0.135%
13	7.763	964	965	971	rVB3	22459	17998	1.56%	0.131%
14	7.881	982	985	987	rBV3	20230	18502	1.60%	0.135%
15	7.975	998	1001	1004	rBV2	34033	30155	2.61%	0.220%
16	8.139	1026	1029	1032	rBV4	16422	21599	1.87%	0.158%
17	8.210	1039	1041	1043	rBV	87851	69918	6.06%	0.510%
18	8.239	1043	1046	1049	rVV	1432870	1134085	98.26%	8.279%
19	8.286	1052	1054	1057	rVB2	80572	72236	6.26%	0.527%
20	8.322	1057	1060	1062	rBV3	24738	23891	2.07%	0.174%
21	8.439	1077	1080	1083	rVB3	27255	20217	1.75%	0.148%
22	8.528	1091	1095	1099	rBV4	52393	66761	5.78%	0.487%
23	8.575	1099	1103	1106	rBV5	18420	27631	2.39%	0.202%
24	8.651	1113	1116	1118	rBV	82329	64899	5.62%	0.474%
25	8.675	1118	1120	1122	rBV2	22467	17073	1.48%	0.125%
26	8.704	1122	1125	1129	rVB5	19781	22928	1.99%	0.167%
27	8.745	1129	1132	1134	rBV4	29369	27212	2.36%	0.199%
28	8.775	1134	1137	1140	rBV4	21708	26163	2.27%	0.191%
29	8.822	1142	1145	1149	rVB3	75199	63327	5.49%	0.462%
30	8.869	1149	1153	1154	rBV4	16490	23713	2.05%	0.173%
31	8.916	1159	1161	1165	rVV3	30477	34100	2.95%	0.249%
32	8.951	1165	1167	1170	rVB	43096	32787	2.84%	0.239%
33	8.986	1170	1173	1175	rBV4	25723	20441	1.77%	0.149%
34	9.016	1175	1178	1180	rBV3	23764	30387	2.63%	0.222%
35	9.051	1182	1184	1188	rVV2	42448	46579	4.04%	0.340%
36	9.104	1191	1193	1194	rBV	27435	24629	2.13%	0.180%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
 Data File : BF126739.D
 Acq On : 29 Jan 2022 01:36
 Operator : CG/JU
 Sample : N1314-01 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-012722

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	9.145	1197	1200	1203	rVB4	34191	43388	3.76%	0.317%
38	9.186	1203	1207	1210	rBV4	30687	33434	2.90%	0.244%
39	9.228	1211	1214	1216	rVV3	34846	34471	2.99%	0.252%
40	9.251	1216	1218	1221	rVV	112933	86623	7.51%	0.632%

41	9.310	1225	1228	1233	rBV	552327	498269	43.17%	3.637%
42	9.386	1238	1241	1244	rBV2	91702	91603	7.94%	0.669%
43	9.463	1252	1254	1257	rVB4	34611	29516	2.56%	0.215%
44	9.510	1259	1262	1266	rVB4	24232	25400	2.20%	0.185%
45	9.575	1271	1273	1279	rBV2	57115	85096	7.37%	0.621%

46	9.651	1283	1286	1289	rVV4	90274	114192	9.89%	0.834%
47	9.710	1293	1296	1299	rVV2	154828	164874	14.28%	1.204%
48	9.769	1303	1306	1308	rBV2	60273	53362	4.62%	0.390%
49	9.816	1312	1314	1316	rVB	27321	20419	1.77%	0.149%
50	9.863	1318	1322	1324	rBV5	54353	51593	4.47%	0.377%

51	9.916	1324	1331	1334	rBV2	76809	99678	8.64%	0.728%
52	9.957	1336	1338	1340	rBV2	16503	19002	1.65%	0.139%
53	9.998	1340	1345	1349	rVV	1349221	1143824	99.10%	8.350%
54	10.027	1349	1350	1354	rVB3	24507	20940	1.81%	0.153%
55	10.098	1359	1362	1367	rBV2	46145	63168	5.47%	0.461%

56	10.145	1367	1370	1374	rBV4	35988	60591	5.25%	0.442%
57	10.180	1374	1376	1377	rVV	34116	31327	2.71%	0.229%
58	10.198	1377	1379	1383	rVV2	58789	63146	5.47%	0.461%
59	10.239	1383	1386	1391	rVV2	80475	83548	7.24%	0.610%
60	10.316	1395	1399	1401	rBV2	60828	65702	5.69%	0.480%

61	10.339	1401	1403	1406	rVV4	30008	29770	2.58%	0.217%
62	10.422	1410	1417	1419	rBV2	79159	115756	10.03%	0.845%
63	10.451	1419	1422	1424	rBV3	26823	24432	2.12%	0.178%
64	10.545	1432	1438	1440	rBV5	29826	49801	4.31%	0.364%
65	10.616	1448	1450	1451	rBV	54666	40921	3.55%	0.299%

66	10.639	1451	1454	1456	rVV	113866	120627	10.45%	0.881%
67	10.692	1460	1463	1468	rVB6	34817	43357	3.76%	0.317%
68	10.763	1472	1475	1476	rBV	41423	29501	2.56%	0.215%
69	10.786	1476	1479	1484	rVB	288725	231746	20.08%	1.692%
70	10.910	1495	1500	1503	rBV2	132042	180424	15.63%	1.317%

71	10.986	1510	1513	1516	rVB2	31093	24414	2.12%	0.178%
72	11.086	1527	1530	1534	rBV5	35265	51910	4.50%	0.379%
73	11.127	1534	1537	1540	rVV3	56932	68862	5.97%	0.503%
74	11.157	1540	1542	1544	rVV3	23424	19100	1.65%	0.139%
75	11.180	1544	1546	1549	rVB4	22364	17475	1.51%	0.128%

76	11.222	1550	1553	1554	rVV2	19952	21825	1.89%	0.159%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
 Data File : BF126739.D
 Acq On : 29 Jan 2022 01:36
 Operator : CG/JU
 Sample : N1314-01 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-012722

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	11.239	1554	1556	1563	rVV5	40058	56808	4.92%	0.415%
78	11.292	1563	1565	1568	rVV4	23415	23471	2.03%	0.171%
79	11.345	1571	1574	1576	rVV	69474	63221	5.48%	0.462%
80	11.374	1576	1579	1586	rVB3	106699	134484	11.65%	0.982%
81	11.492	1595	1599	1602	rBV	1377666	1154186	100.00%	8.426%
82	11.516	1602	1603	1606	rVB	101969	62507	5.42%	0.456%
83	11.721	1636	1638	1641	rBV4	33690	35187	3.05%	0.257%
84	11.774	1644	1647	1650	rVB	49838	42938	3.72%	0.313%
85	11.821	1653	1655	1661	rVB4	27018	34828	3.02%	0.254%
86	11.998	1682	1685	1688	rBV3	52389	65412	5.67%	0.478%
87	12.021	1688	1689	1694	rVB	49065	32562	2.82%	0.238%
88	12.104	1701	1703	1706	rBV2	31758	29738	2.58%	0.217%
89	12.180	1714	1716	1719	rBV2	43617	45878	3.97%	0.335%
90	12.468	1763	1765	1767	rBV2	24511	22056	1.91%	0.161%
91	12.545	1775	1778	1780	rBV	46133	43459	3.77%	0.317%
92	12.574	1780	1783	1787	rVB2	55572	61548	5.33%	0.449%
93	12.710	1803	1806	1809	rBV	152665	124408	10.78%	0.908%
94	12.945	1843	1846	1852	rVB2	155760	170366	14.76%	1.244%
95	13.080	1866	1869	1872	rBV	589215	468757	40.61%	3.422%
96	13.304	1905	1907	1910	rBV2	53318	51827	4.49%	0.378%
97	13.645	1963	1965	1969	rBV2	74441	97125	8.42%	0.709%
98	14.145	2046	2050	2053	rBV	1135457	1057249	91.60%	7.718%
99	14.927	2181	2183	2186	rVB	150496	118747	10.29%	0.867%
100	15.674	2306	2310	2321	rVB2	593554	1066662	92.42%	7.787%




Sum of corrected areas: 13698454

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126739.D
Acq On : 29 Jan 2022 01:36
Operator : CG/JU
Sample : N1314-01 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-012722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

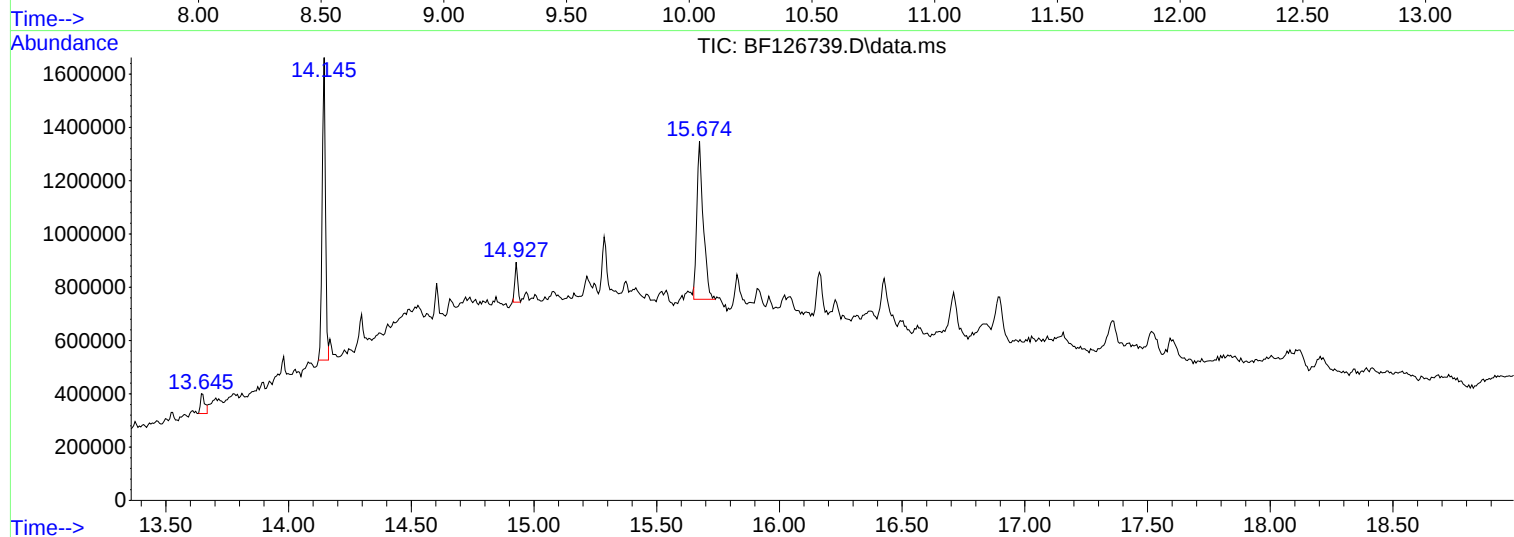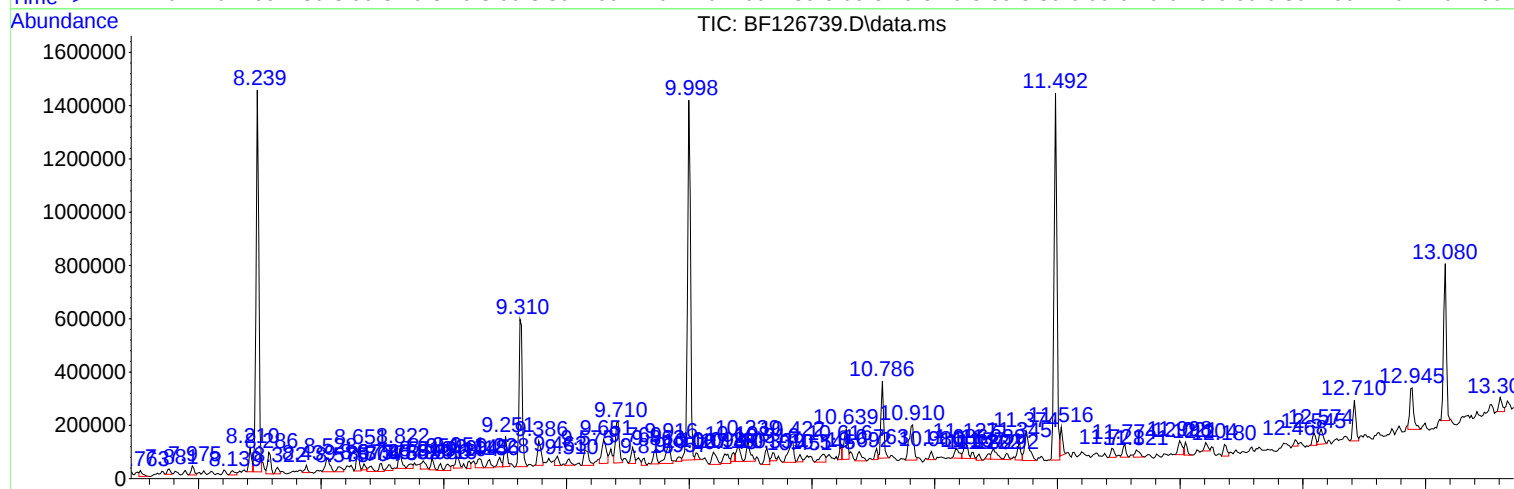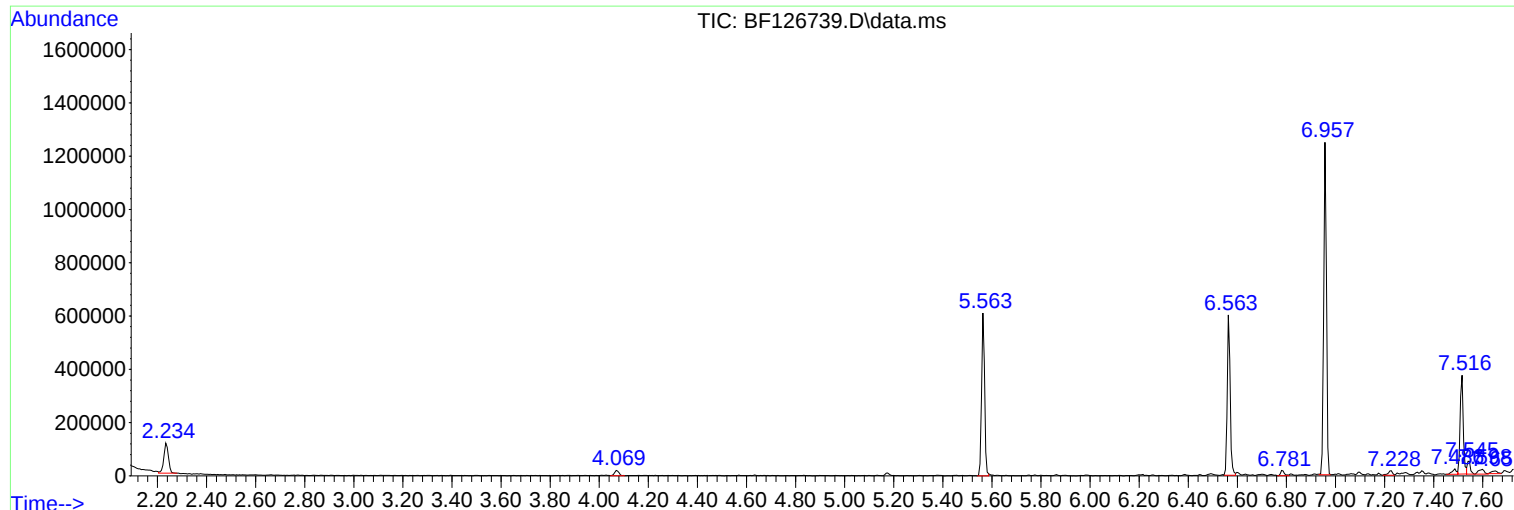

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126739.D
Acq On : 29 Jan 2022 01:36
Operator : CG/JU
Sample : N1314-01 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-012722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126739.D
Acq On : 29 Jan 2022 01:36
Operator : CG/JU
Sample : N1314-01 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-012722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------